



Brookhaven
National Laboratory

BNL-104096-2014-TECH

AGS.SN220;BNL-104096-2014-IR

Latest Results from Studies of Induced Radioactivity

K. A. Brown

January 1987

Collider Accelerator Department
Brookhaven National Laboratory

U.S. Department of Energy

USDOE Office of Science (SC)

Notice: This technical note has been authored by employees of Brookhaven Science Associates, LLC under Contract No. DE-AC02-76CH00016 with the U.S. Department of Energy. The publisher by accepting the technical note for publication acknowledges that the United States Government retains a non-exclusive, paid-up, irrevocable, world-wide license to publish or reproduce the published form of this technical note, or allow others to do so, for United States Government purposes.

DISCLAIMER

This report was prepared as an account of work sponsored by an agency of the United States Government. Neither the United States Government nor any agency thereof, nor any of their employees, nor any of their contractors, subcontractors, or their employees, makes any warranty, express or implied, or assumes any legal liability or responsibility for the accuracy, completeness, or any third party's use or the results of such use of any information, apparatus, product, or process disclosed, or represents that its use would not infringe privately owned rights. Reference herein to any specific commercial product, process, or service by trade name, trademark, manufacturer, or otherwise, does not necessarily constitute or imply its endorsement, recommendation, or favoring by the United States Government or any agency thereof or its contractors or subcontractors. The views and opinions of authors expressed herein do not necessarily state or reflect those of the United States Government or any agency thereof.

AGS Studies Report

Date(s) 1/4 - 1/27/87 Time(s) _____
Experimenter(s) K.A. Brown and M. Tanaka
Reported by K.A. Brown
Subject Latest Results from Studies of Induced Radioactivity

In Accelerator Division Technical Note No. 246 we described the relationship between measured radiation dose and beam loss. Using the approximation,

$$D = k \xi \ln(1 + T/t),$$

we calculated values of k for high energy protons in the AGS (at which D was the dose measured at a standard distance of 12 inches). Values were found for the FEB run in 1985, the FEB run in 1986, and the SEB run in 1986. This January we ran SEB and during the 1/27-28 maintenance, Health Physics did a full ring survey and we calculated values for k for this run.

In December, 1986, we began collecting beam intensity data and beam hours data more frequently. A program was written which sampled the beam current transformer every hour at different times (ICBM, 3CBM, CBM, and XCBM times) and sampled the CE010 SEC every hour. This data allows a better resolution on the amount of beam lost during the run. Also, more attention was paid to the number of hours there was beam in the machine and the number of hours there was extracted beam.

We also found a few minor errors in the calculations of k published in Accelerator Division Technical Note No. 264. Basically, the errors involved keeping the method of calculation more consistent for each point.

Figure I shows the energy dependence of k . Injection is approximately 200 MeV, transition is approximately 8 GeV, and extraction is approximately 30 GeV.

Figure II shows k for injection for the four different runs. Figure III shows k for transition for the four different runs. Figure IV shows k for extraction for the four different runs.

Figure V shows the capture efficiency over the month of January. Figure VI shows the acceleration and transition efficiencies. Figure VII shows the extraction efficiency. Note that the extraction efficiency is taken as CE_{010}/X_{CBM} and does not include any calibration constant.

Also included is a copy of the HP ring survey taken on January 27, 1987. Of particular concern are the unexpected high levels seen in the H11 region.

FIGURE I

LOG (k) VS TIME IN CYCLE

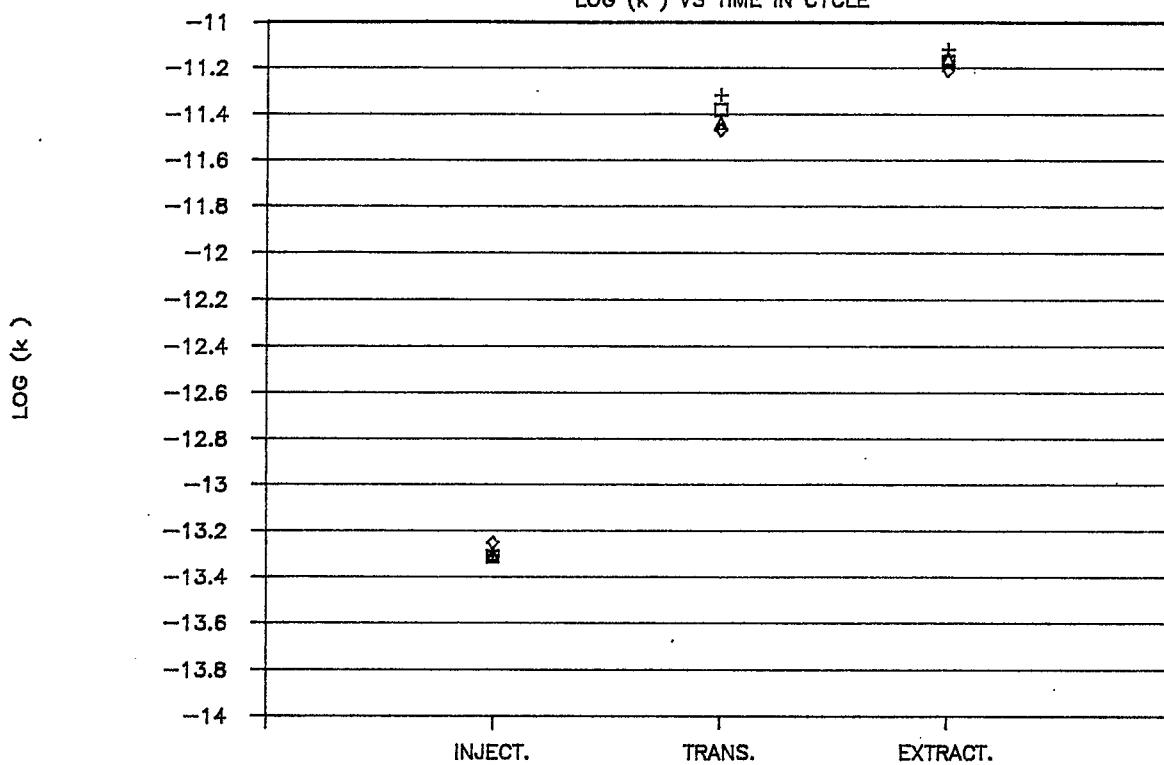


FIGURE II

VALUE OF k VS RUN: INJECTION

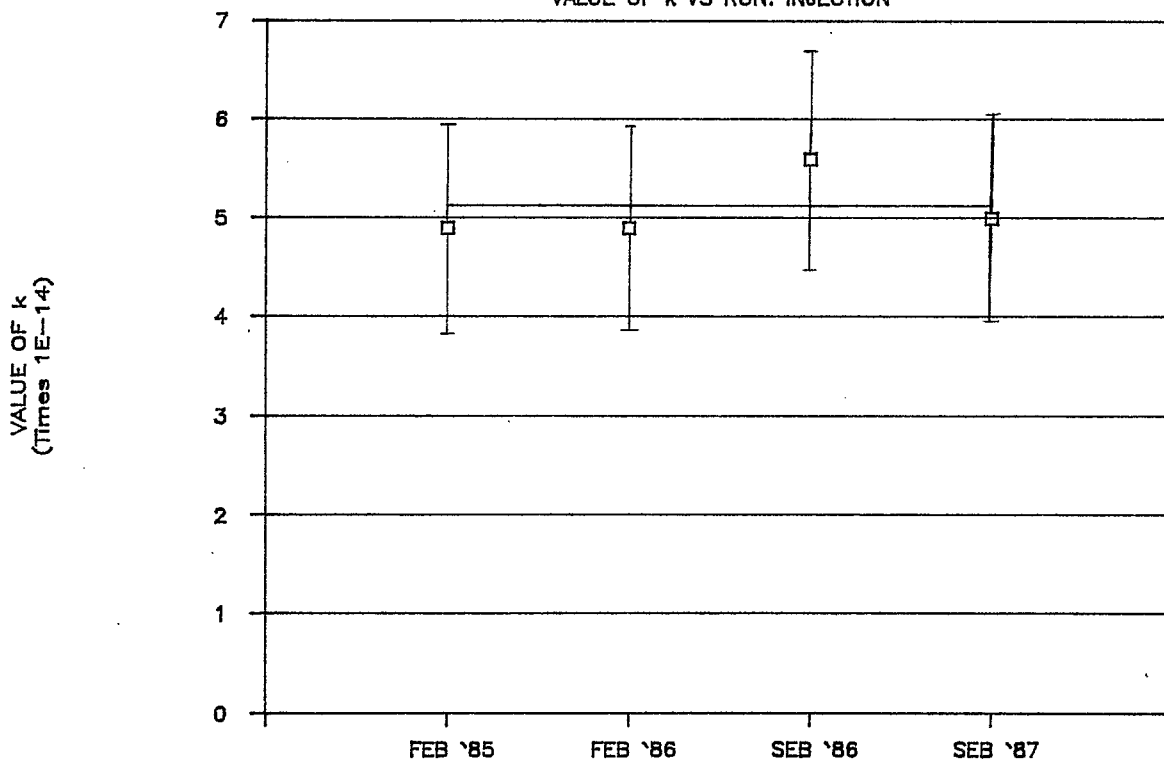


FIGURE III

VALUE OF k VS RUN: TRANSITION

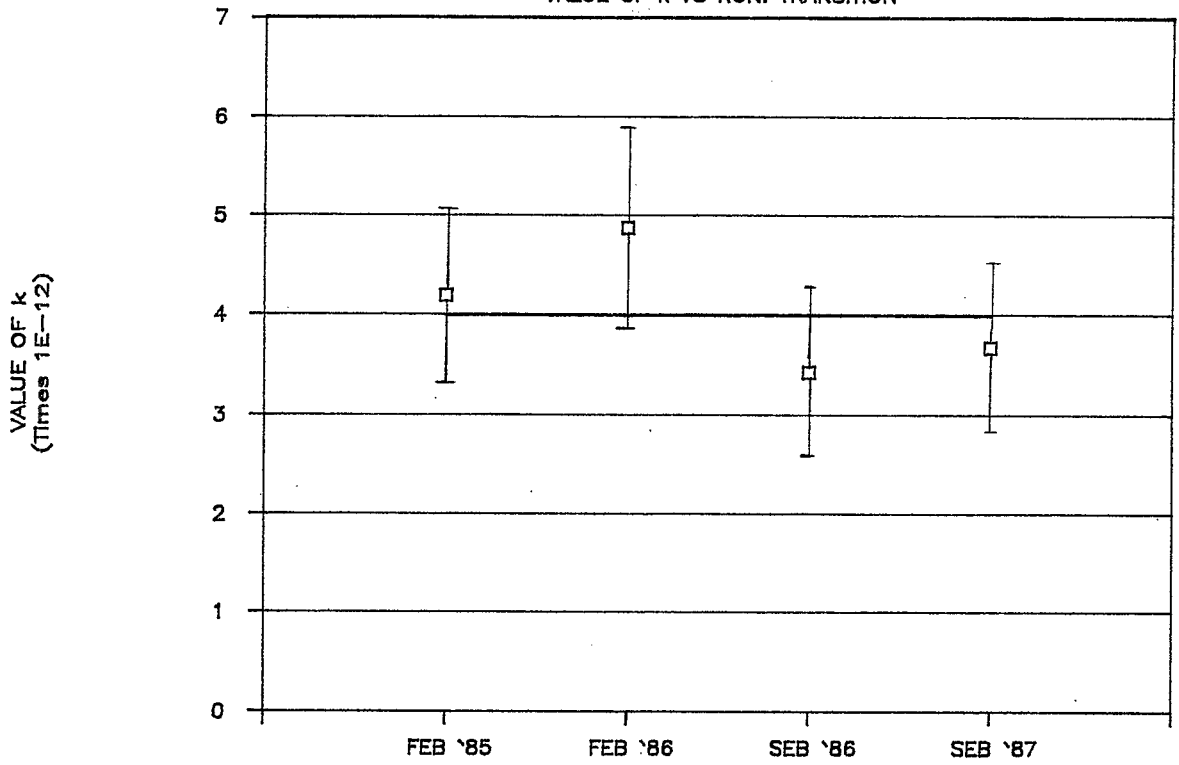


FIGURE IV

VALUE OF k VS RUN: EXTRACTION

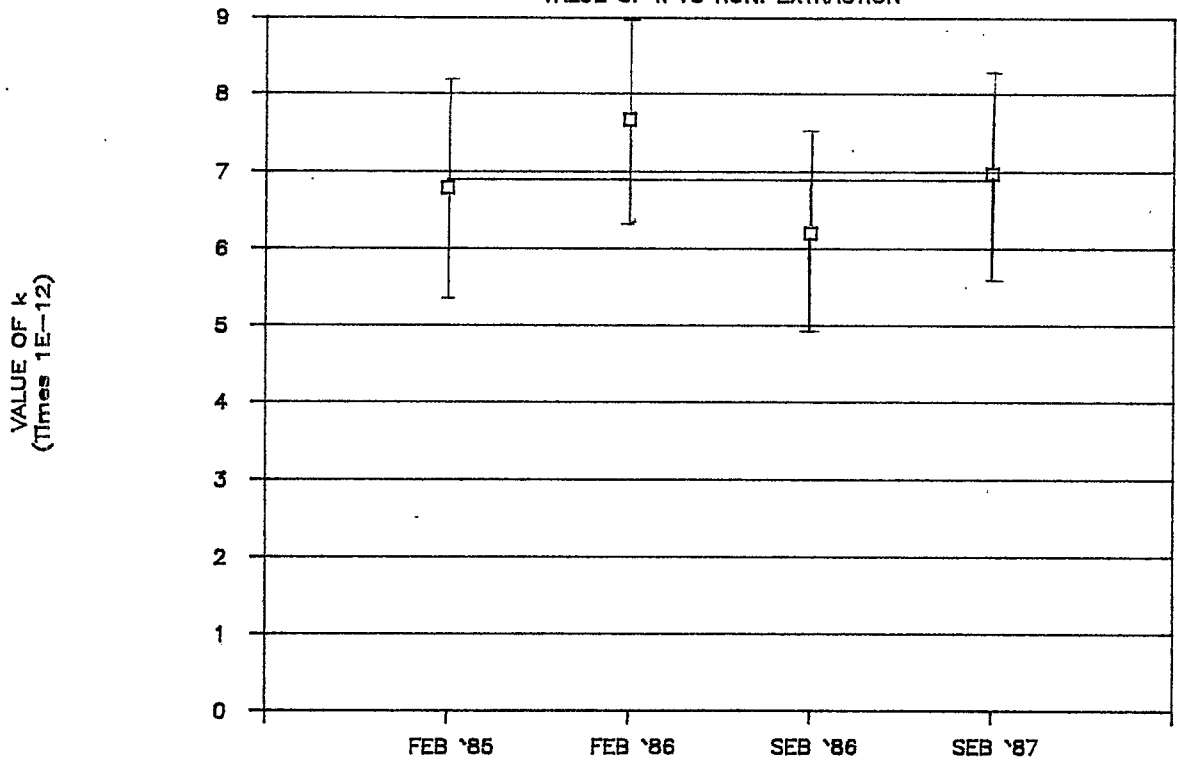


FIGURE V

CAPTURE EFF. DURING JANUARY

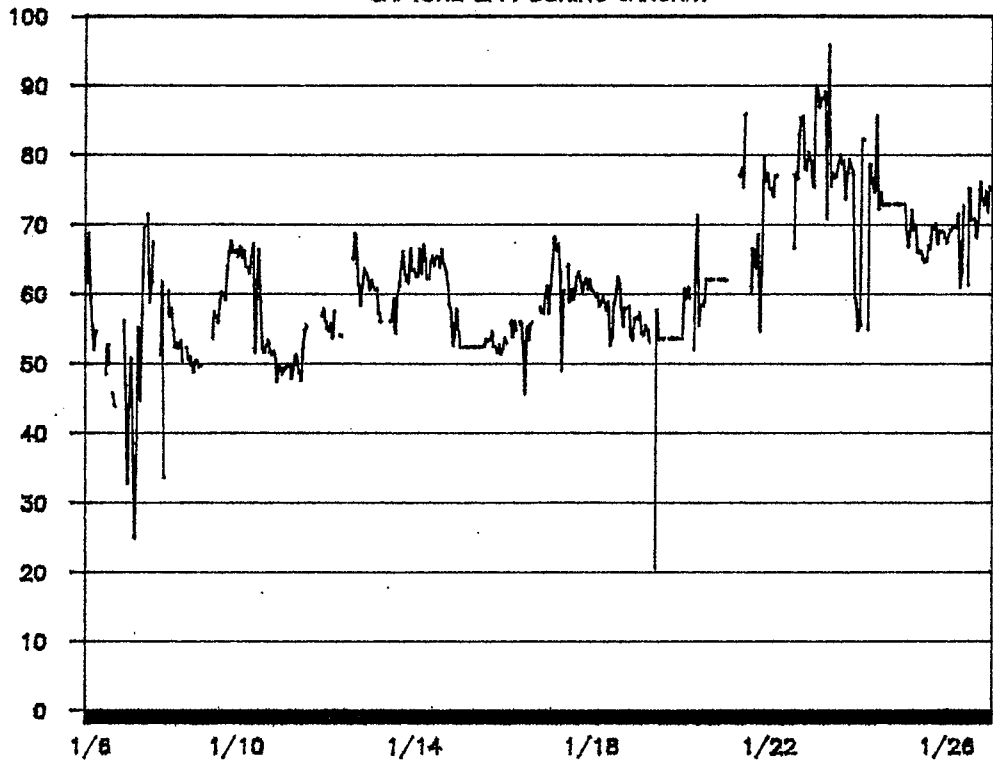


FIGURE VI

ACCEL. & TRAN. EFF. DURING JANUARY


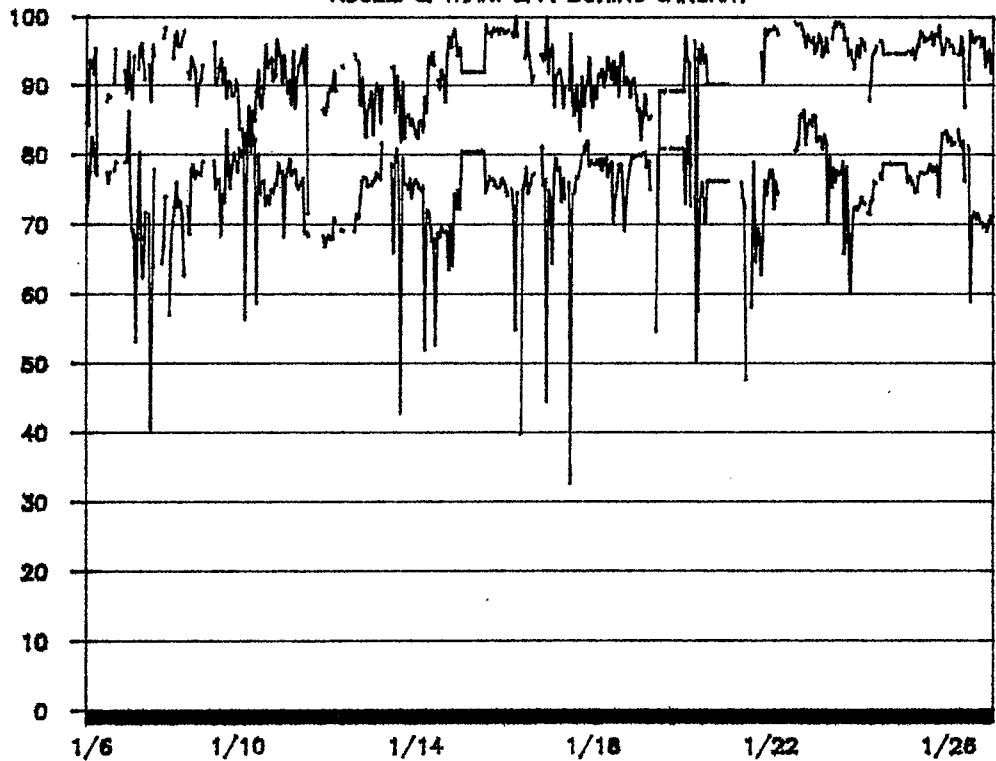



FIGURE VII

EXTRACTION EFF. DURING JANUARY

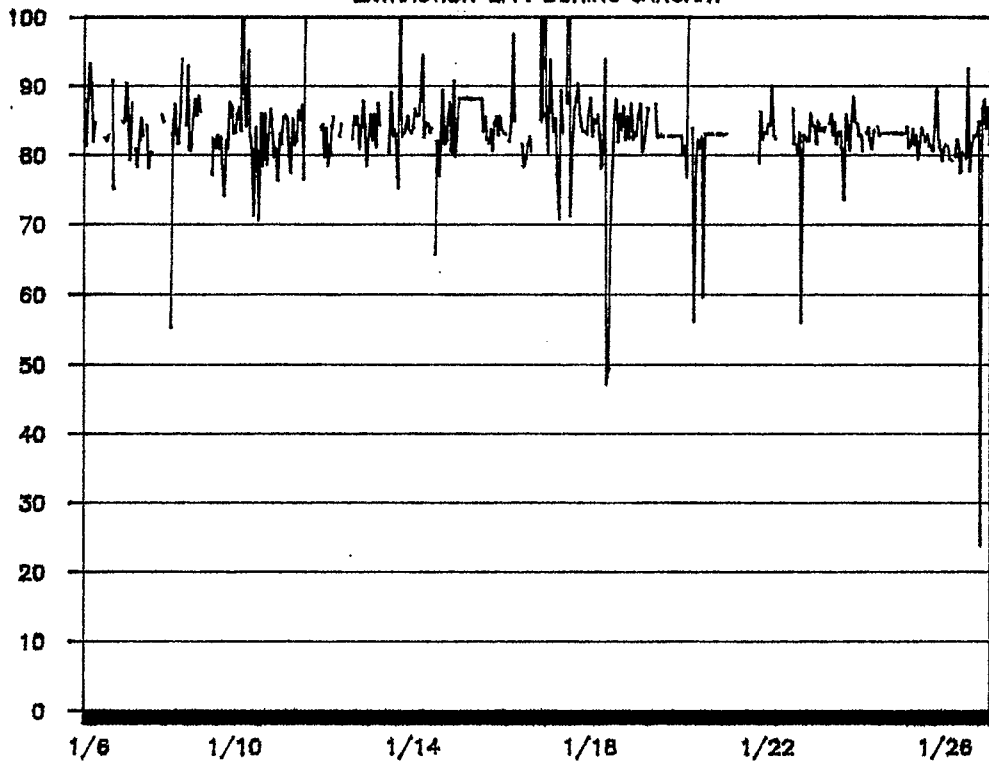

HP RING SURVEY

(27-Jan-87) - (01-Dec-86)

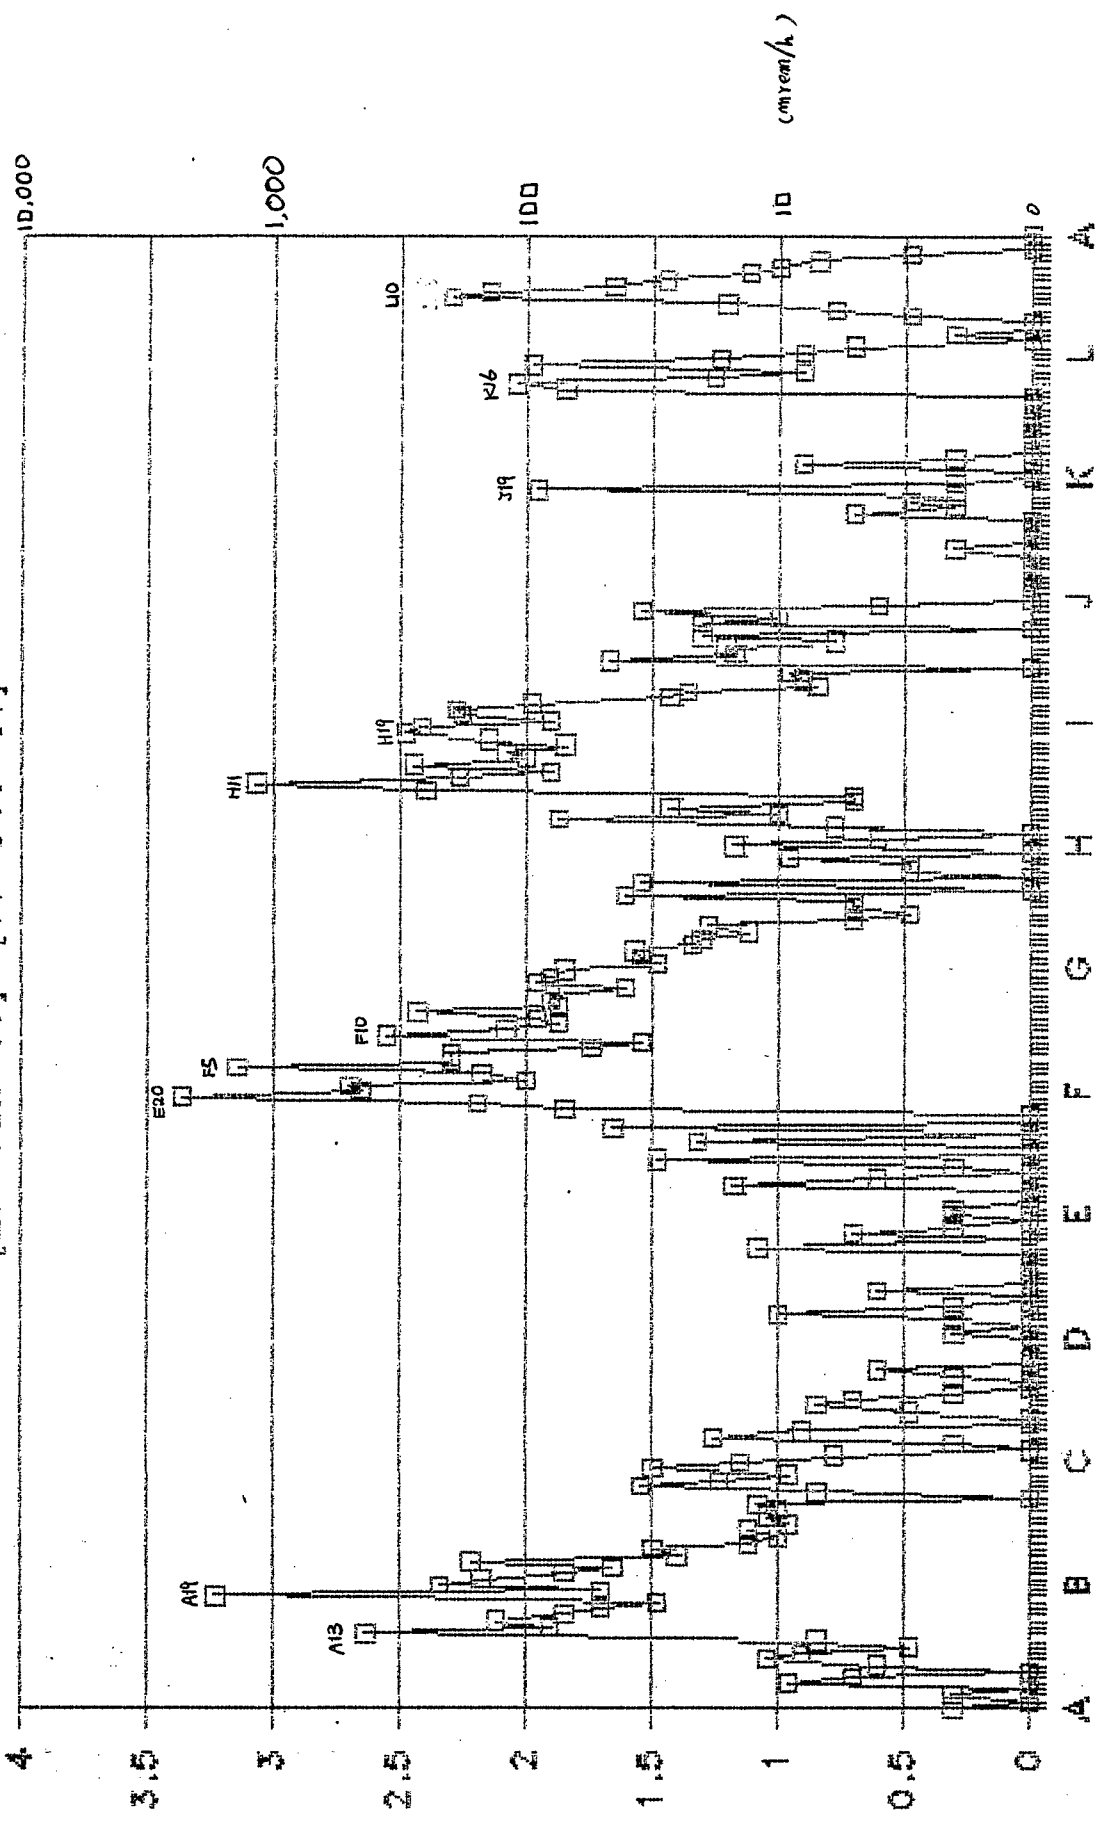

Superperiods A-01 to L-20
□ Out at 12"

(4 / 1011) 007

Scanned