

## ELECTROSTATIC INFLECTOR

L. E. Repeta

July 1969

Collider Accelerator Department  
**Brookhaven National Laboratory**

**U.S. Department of Energy**

USDOE Office of Science (SC)

Notice: This technical note has been authored by employees of Brookhaven Science Associates, LLC under Contract No. AT-30-2-GEN-16 with the U.S. Department of Energy. The publisher by accepting the technical note for publication acknowledges that the United States Government retains a non-exclusive, paid-up, irrevocable, world-wide license to publish or reproduce the published form of this technical note, or allow others to do so, for United States Government purposes.

## **DISCLAIMER**

This report was prepared as an account of work sponsored by an agency of the United States Government. Neither the United States Government nor any agency thereof, nor any of their employees, nor any of their contractors, subcontractors, or their employees, makes any warranty, express or implied, or assumes any legal liability or responsibility for the accuracy, completeness, or any third party's use or the results of such use of any information, apparatus, product, or process disclosed, or represents that its use would not infringe privately owned rights. Reference herein to any specific commercial product, process, or service by trade name, trademark, manufacturer, or otherwise, does not necessarily constitute or imply its endorsement, recommendation, or favoring by the United States Government or any agency thereof or its contractors or subcontractors. The views and opinions of authors expressed herein do not necessarily state or reflect those of the United States Government or any agency thereof.

Accelerator Department  
BROOKHAVEN NATIONAL LABORATORY  
Associated Universities, Inc.  
Upton, New York

AGS DIVISION TECHNICAL NOTE

No. 62

L.E. Repeta and V.J. Buchanan  
July 8, 1969

ELECTROSTATIC INFLECTOR

Introduction

Multiturn injection has been used at the AGS since August 1964 and has been accomplished by using an electrostatic inflector and associate equipment.

The proton beam leaves the linear accelerator on an optic axis that lies on the median plane of the AGS ring. The beam moves along the axis of the beam transport, which is approximately 4-in. outside a tangent line to the AGS. As the beam moves along this flight path, it is deflected toward the ring. The final tangency of the linac beam to the AGS ring is accomplished by the electrostatic inflector.

Mechanical Design

The inflector is located at the edge of the usable machine aperture at the 10 ft straight section "L-20". The major components of the inflector are shown in a cross sectional view in Fig. 1. The main assembly drawing is D07-M-5103-5, and anyone interested in greater detail should refer to this drawing.

A simplified plan view, with cover removed, is shown in Fig. 2. The sub-base is accurately surveyed in position relative to the line joining the magnet sockets ( $S_0$ ) of the "L-20" and "A-1" AGS main ring magnets. The inflector sub-assembly is accurately positioned, relative to the sub-base,

VIEW LOOKING UPSTREAM

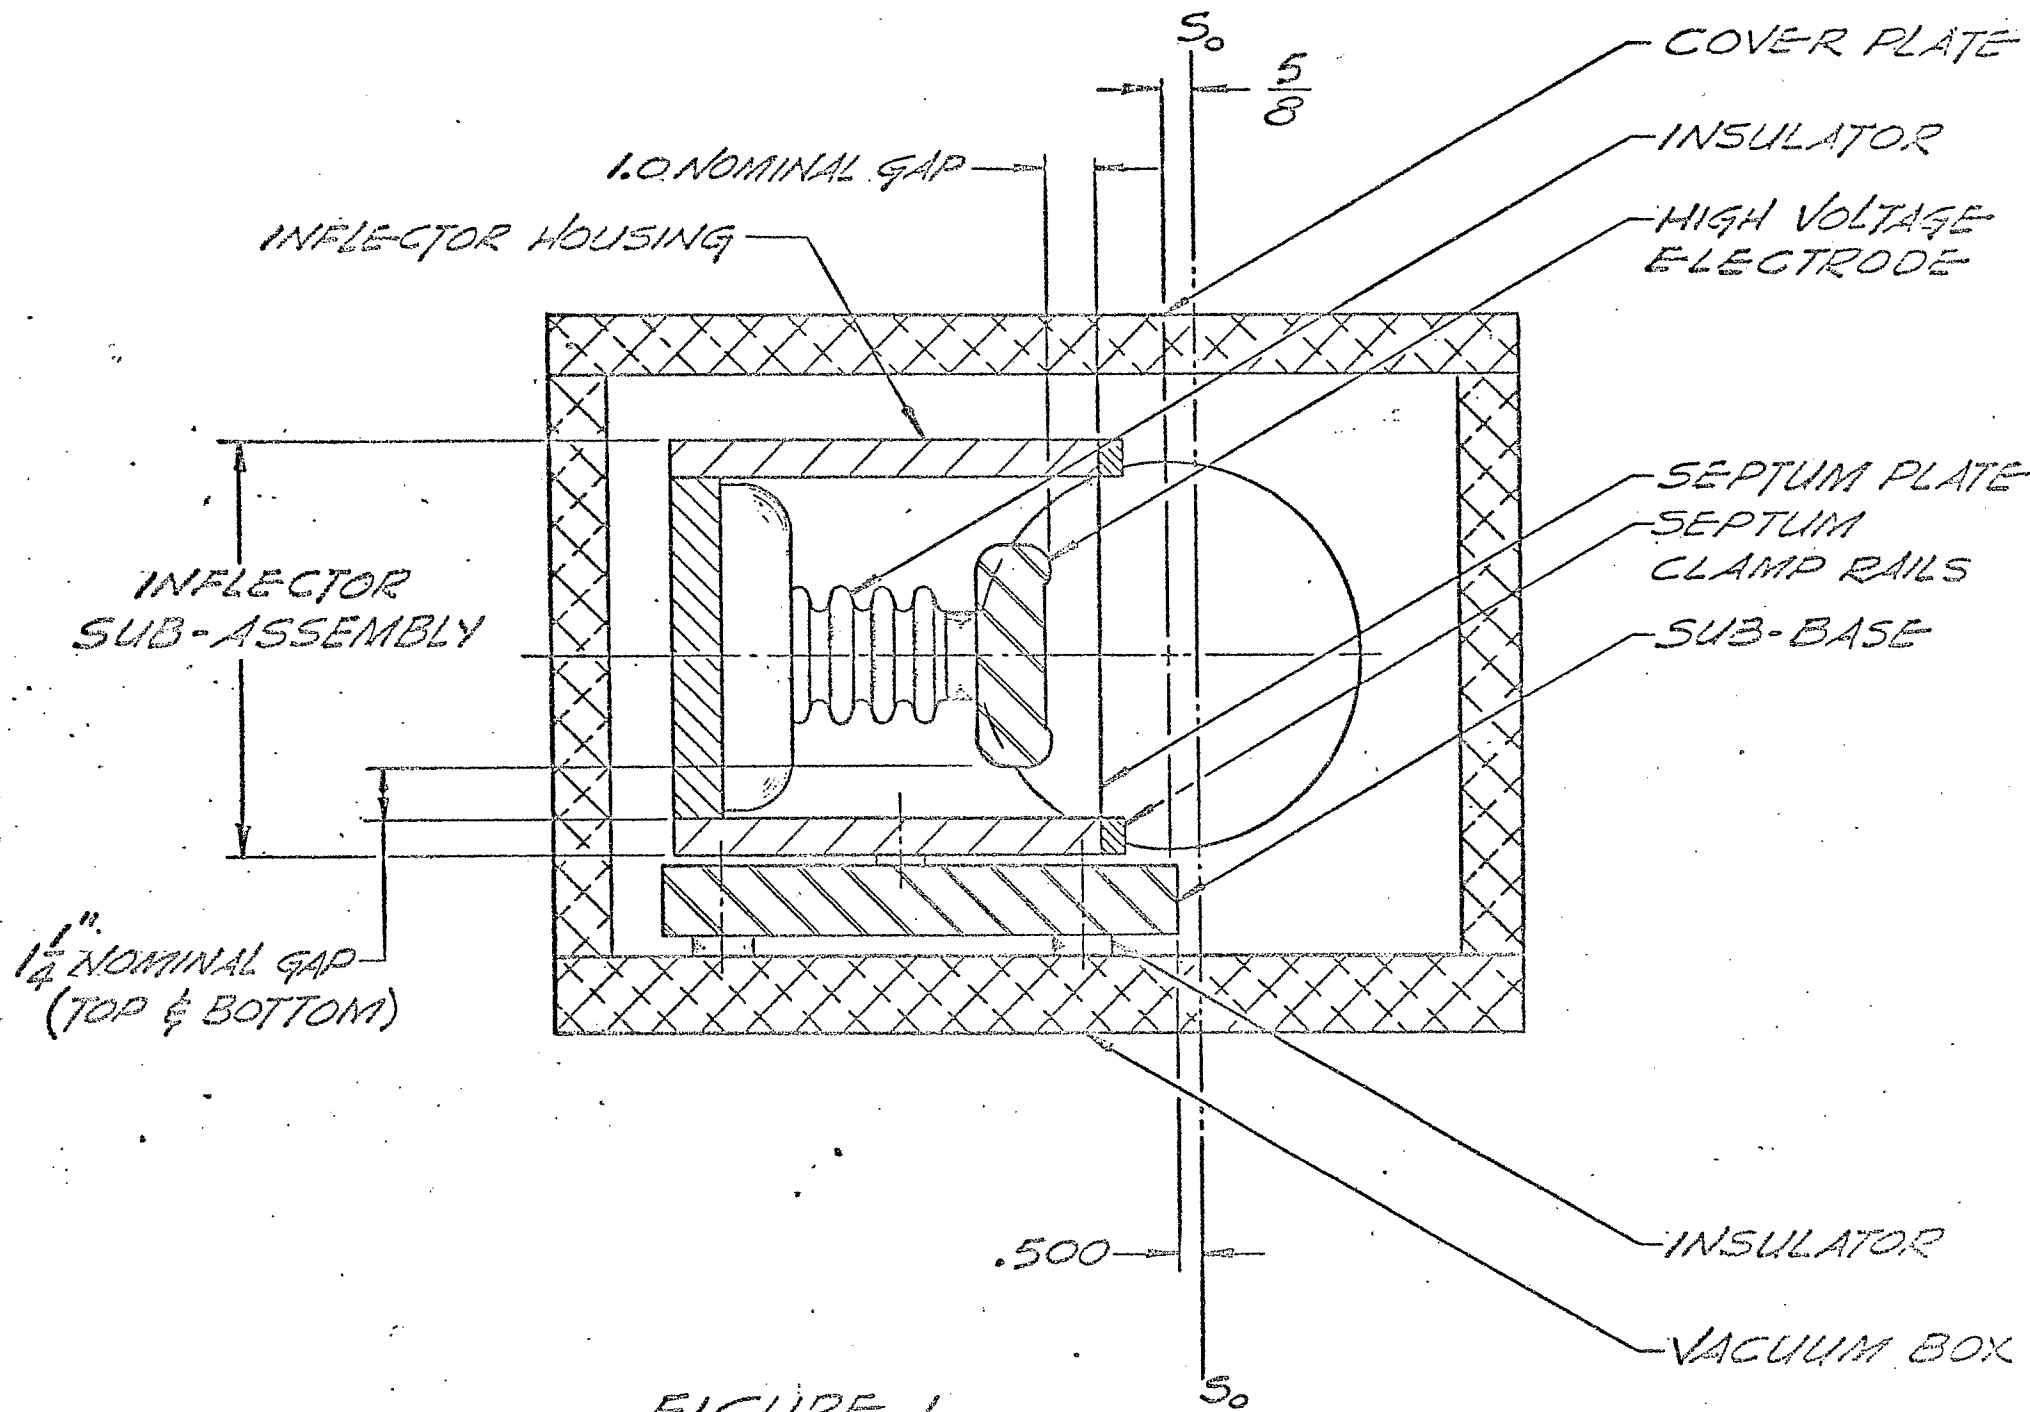


FIGURE 1

through the use of three gage blocks as noted in the figure. The use of these gage blocks facilitates accurate location without survey and insures accurate repositioning of the inflector sub-assembly, after it has been removed for maintenance, with minimum effort and time.

The high voltage electrode is 60-in. long and is made from 6061-T6 aluminum alloy highly polished all over. The electrode front face shape, shown in Fig. 3 was optimized by making equi-potential plots on high resistance paper of ten times size cross sections. The normal running voltage is a negative 45 kV.

Shown in Fig. 4 is a two piece copper shield block that is fastened to, and insulated from, the inflector sub-assembly. In addition, each of the two component pieces are insulated from each other. The function of this block is to--1) act as a collimator for the linac beam, and 2) to provide a protective shield for the outside face of the thin (0.015) septum plate from the orbiting beam. Ceramic beaded, copper signal wire has been run from each piece to a vacuum feed thru located on the front face of the vacuum box; co-ax cable then runs to the AGS Main Control Room. This enables close monitoring for study and evaluation of the signal generated by the entering linac beam "wiping off" on entrance through the opening of the copper block, and the signal generated by the circulating beam "wiping off" on the outside edge of the block as it passes the outside of the inflector.

After several weeks of operation it was found that a thermal breakdown of some of the insulating material (.005 thick "H" film) caused outgassing. This resulted in a serious arcing problem that intermittently tripped the inflector off. The two piece copper shield block was removed and replaced by a one piece shield block. A new split block has been designed and is now ready for installation.

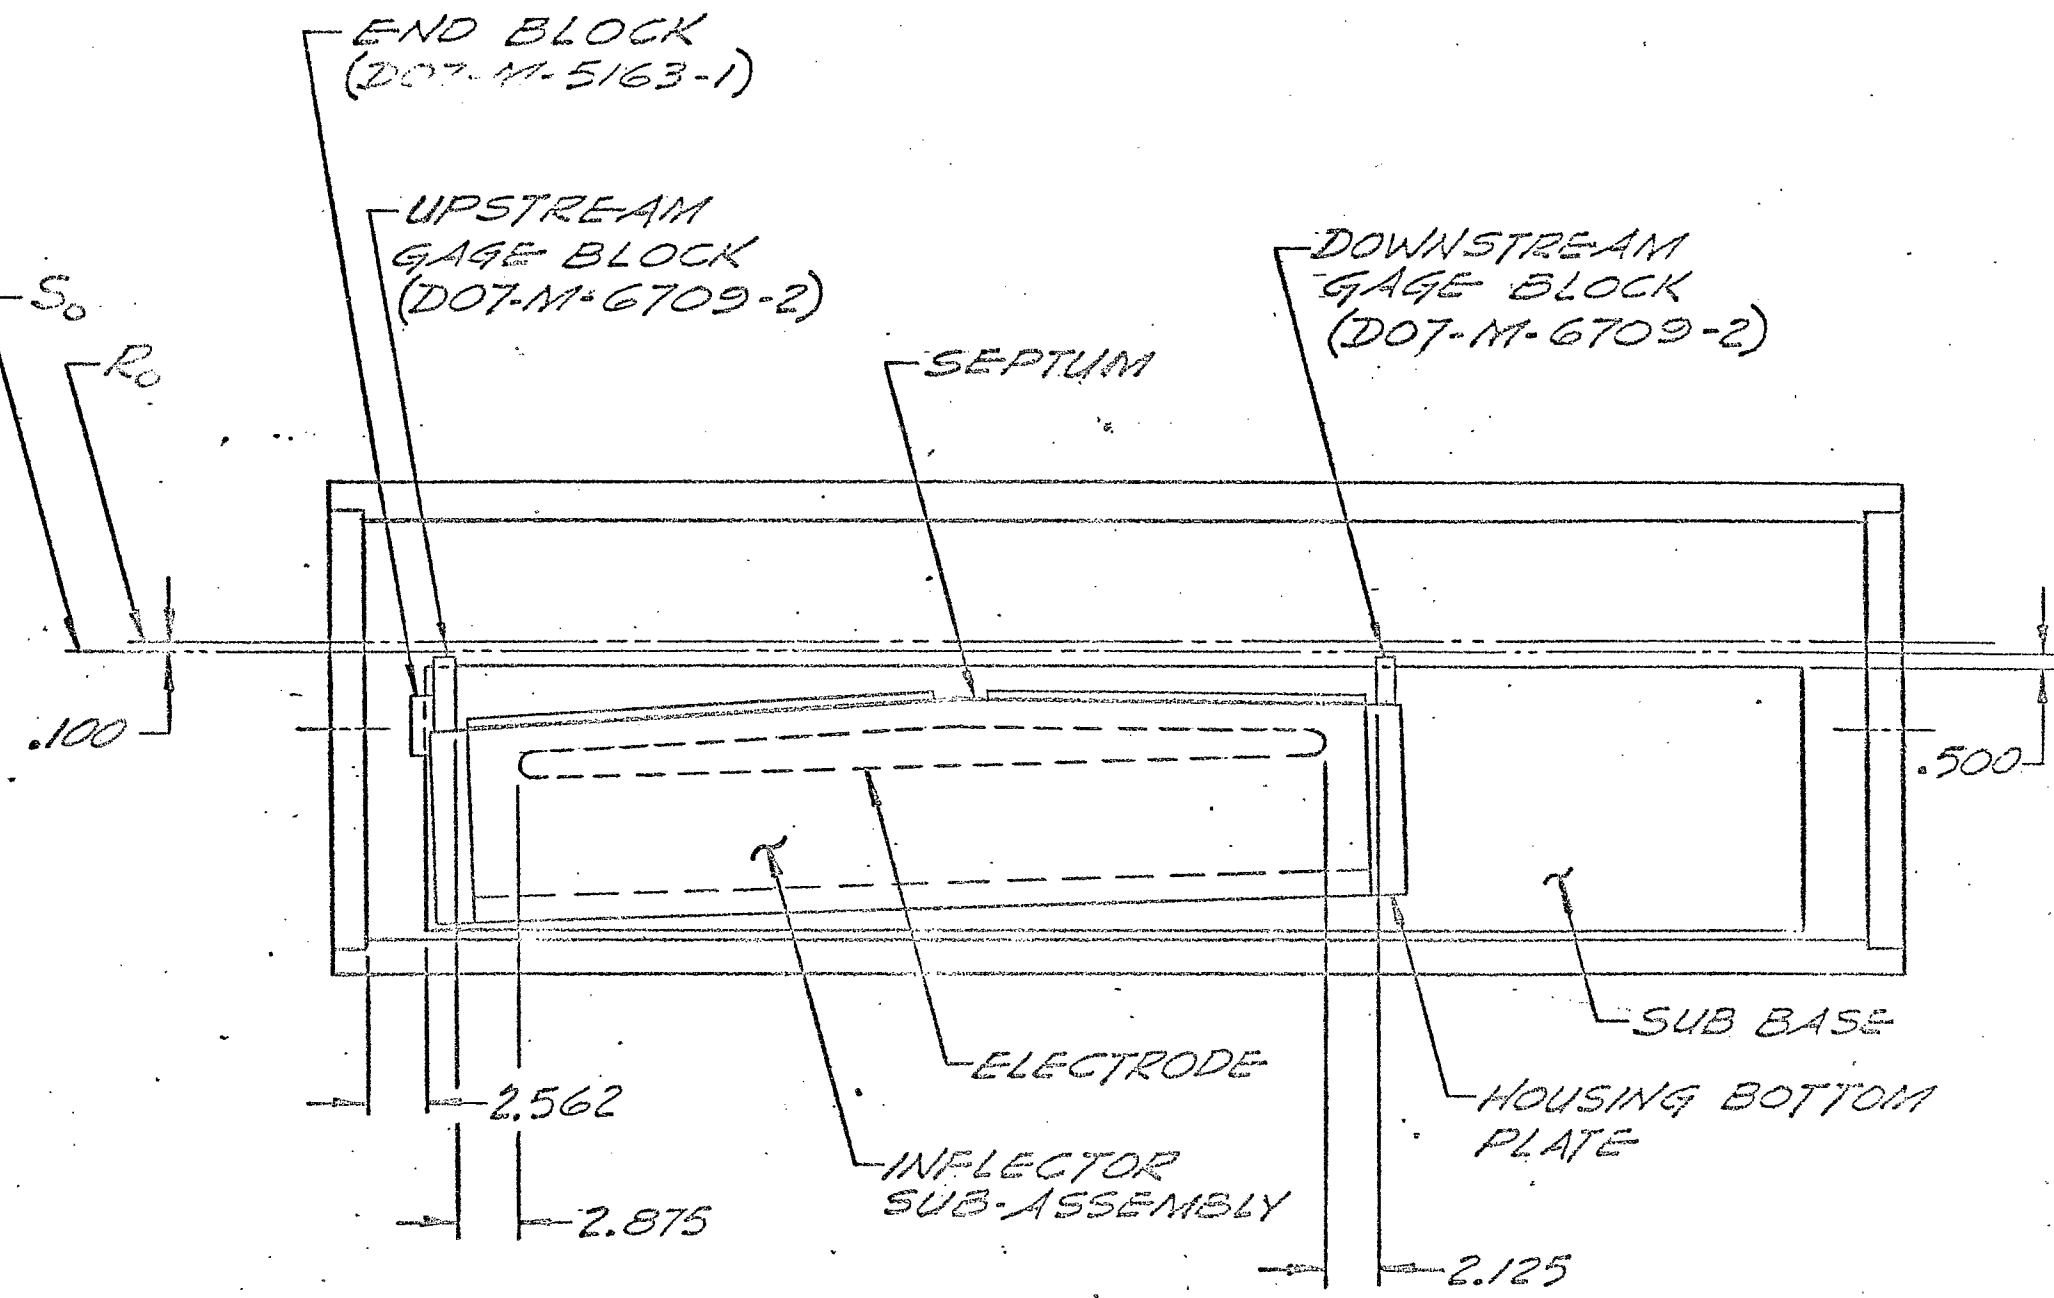


FIGURE 2

The upstream inflector viewing flag and its basic dimensions are shown in Fig. 5. The flag can be remotely positioned to either of the two working positions denoted, or withdrawn within the shadow of the vacuum pipe by activating a 24 volt d.c. linear actuator drive motor from the Main Control Room. A potentiometer readout system, accurately calibrated by the AGS Target Group, enables the machine operator to position the flag in the desired position. The flag is viewed in the Main Control Room via closed circuit television. Operating position #1 is useful when setting up or for studies purposes, but not satisfactory for efficient machine operation because the obstruction presented by the 1/8-in. thick quartz plate "stops" most of the 50 MeV beam. Switching to position #2, the machine operator can center the air gap between the two quartz pieces to the injected beam centerline. The obstruction of the beam due to the flag has been removed and this position also enables the operator to monitor any horizontal movement of the entering beam during normal machine running.

#### Introduction to the Calculations


A computer analysis was made by Dr. A.W. Maschke to determine the initial parameters to be used. A 22 milliradian entrance angle, directed toward the center of the AGS machine, resulted in an offset from the computer coordinate line to the injection line of 2.904 inches (see Fig. 6). The high voltage electrode was to be 60-in. long and an approach angle of 4 milliradians directed away from the center of the AGS, was to be used. The entrance and approach angles were to be distributed equally over the electrode length.

#### Geometric Position and Attitude

Sign convention:

Positive (+) denotes increasing radius and,

Negative (-) denotes decreasing radius (toward the center of the AGS ring).

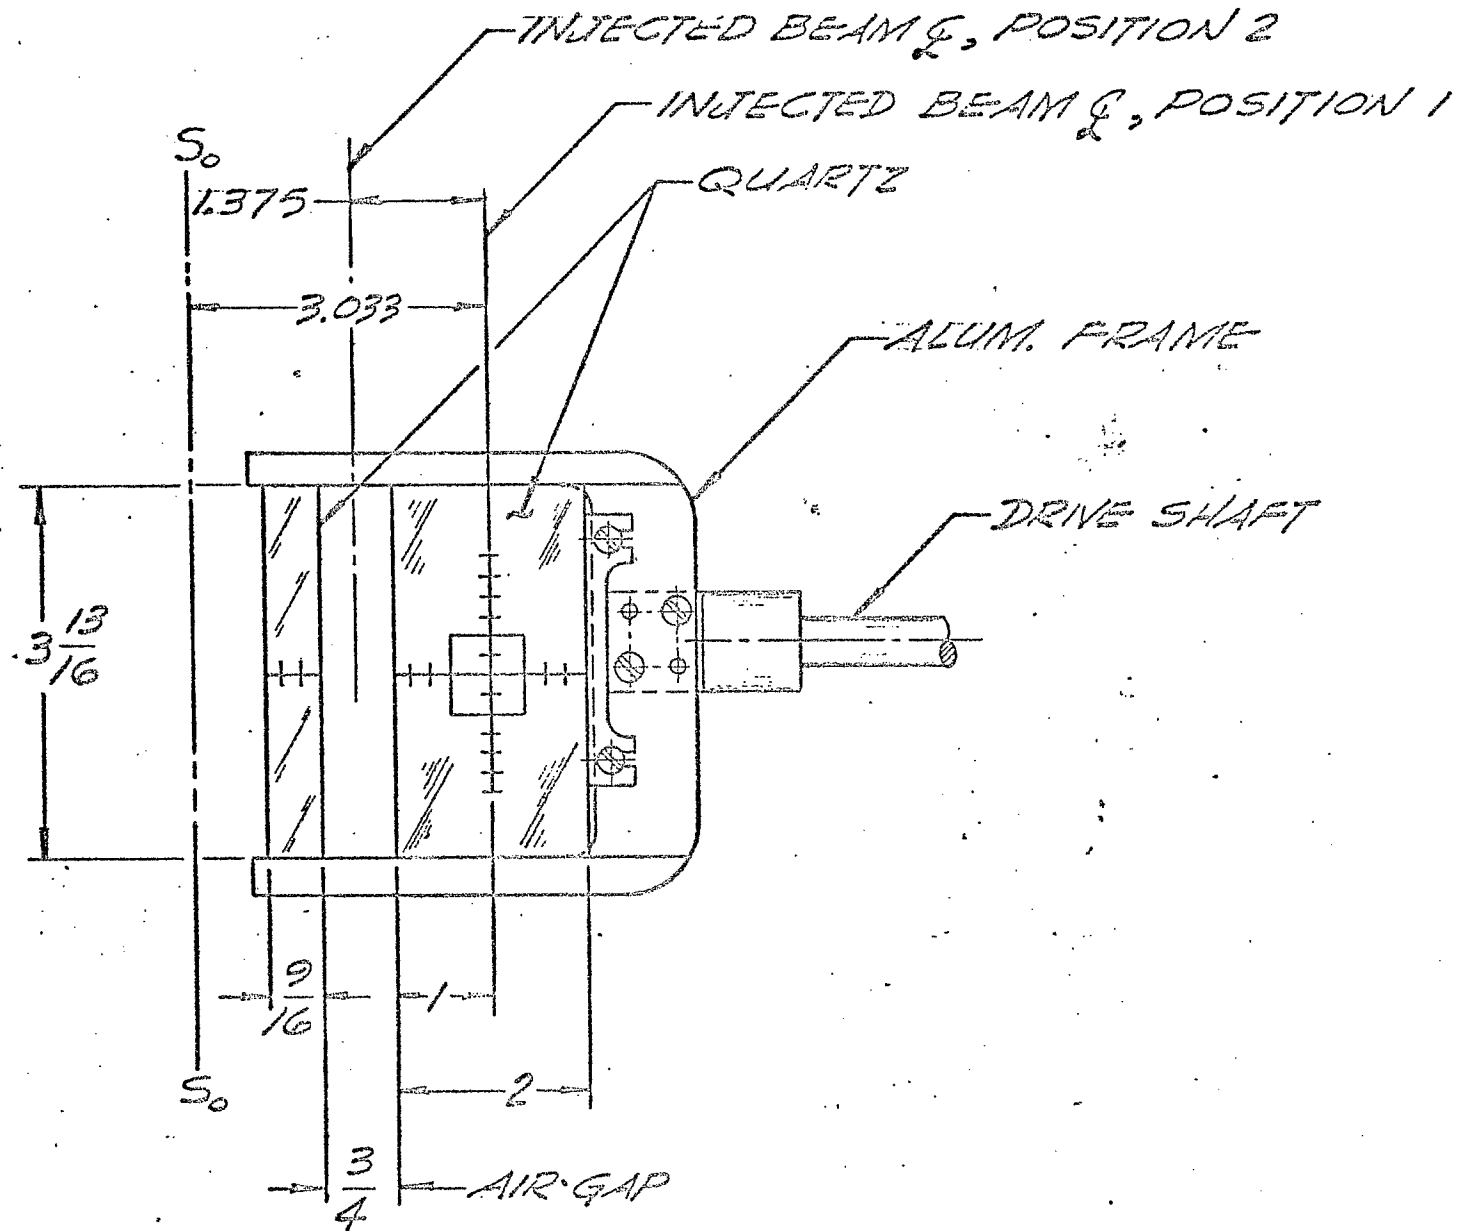

UPSTREAM INFECTOR FLAG (DOT-M-6711-3)  
 VIEW LOOKING DOWNSTREAM

FIGURE 5



Refer to Fig. 6.

From the beam program coordinate line to the line joining the magnet sockets ( $S_0$ ) as taken from drawing D05-412-2.

$$y_1 = 0.035$$

From the beam program coordinate line to an extension of the vacuum chamber centerline in "L-20" (computer coordinate line)

$$y_2 = 12'' (\tan 0^\circ 36') = 12 (0.01047) =$$

$$\frac{y_2 = 0.126}{0.161}$$

Offset from the computer coordinate line to the injection line as taken from the computer sheet

$$2.904$$

Offset 6-in. downstream at 22 milliradians

$$y_3 = -6.000 (0.022) =$$

$$\frac{y_3 = 0.132}{2.933}$$

Centerline of a 1/2-in. diameter beam will enter the inflector 3/8-in. from the inside face of the septum plate

$$\underline{-0.375}$$

Distance from the socket line to the inside face of the septum at the upstream end of the inflector electrode

$$\boxed{2.558}$$

The electrode gap will go upstream for 30-in. at 22 milliradians

$$-30'' (0.022) =$$

$$\frac{-0.660}{1.898}$$

The electrode gap will then continue upstream for 30-in. at 4 milliradians

$$+30'' (0.004) =$$

$$+0.120$$

The centerline of the beam will leave the gap 1/8-in. closer to the septum plate, graze the septum plate and exit

$$\underline{+0.125}$$

Distance from the socket line to the inside face of the septum at the downstream end of the inflector electrode

$$\boxed{2.143}$$

Refer to Fig. 7.

The septum sheet angle:

$$22 \text{ mR} + 4 \text{ mR} = 26 \text{ mR}; \quad 26 \text{ mR}/2 = 13 \text{ mR}$$

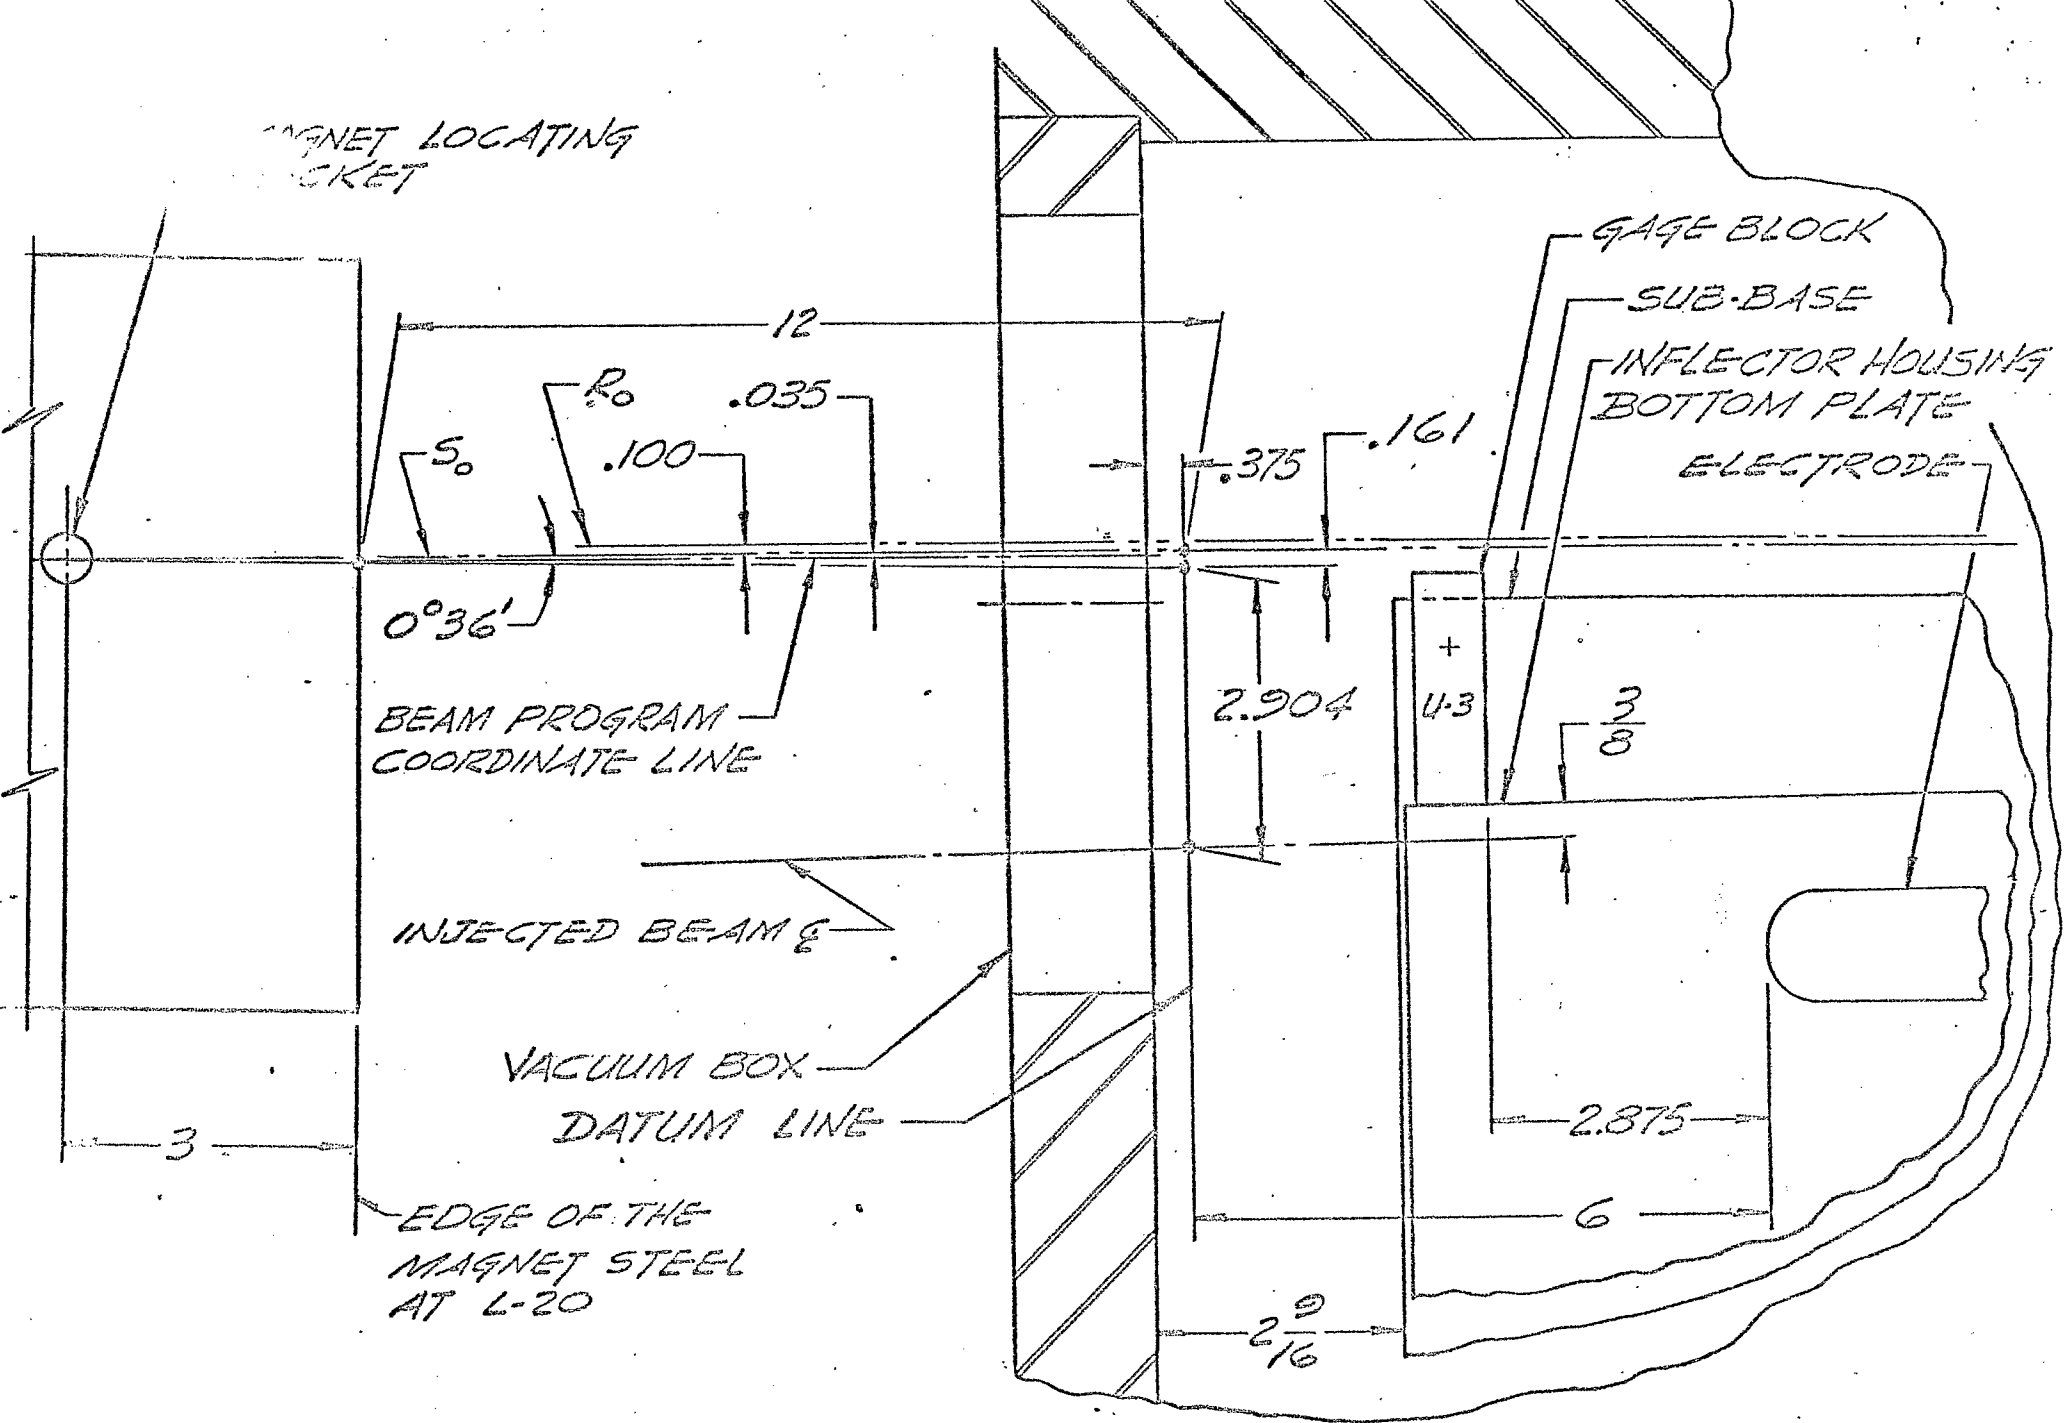


FIGURE 6

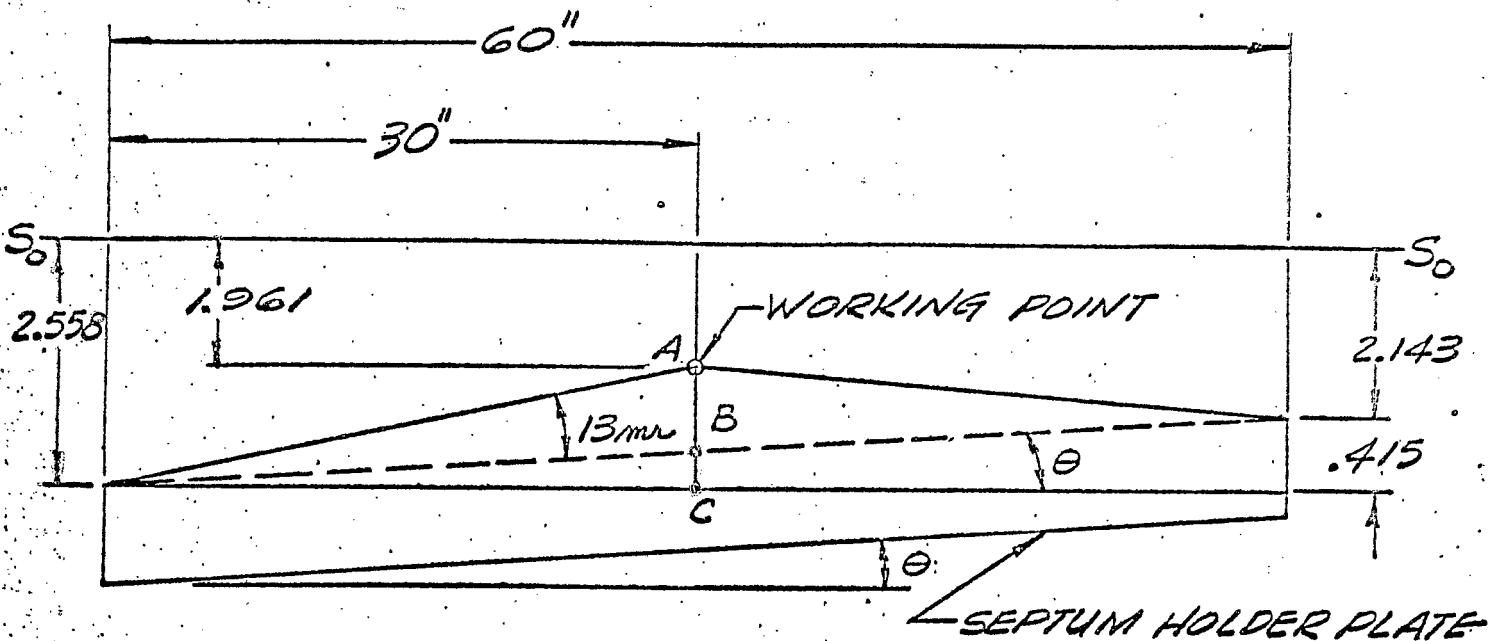


FIGURE 7

THE CALCULATION OF THE ANGLE AT THE BACK OF THE SEPTUM

HOLDER PLATES ( $\theta$  in figure 7).

$$(1) \begin{array}{r} 2.558 \\ -2.143 \\ \hline 0.415 \end{array} \quad (2) \tan \theta = \frac{.415}{60} = 0.006916 \approx 0.007$$

$\therefore$  Let  $\theta = 7$  milliradians

Socket line to the inside of the septum at the upstream end of the electrode 2.558

The septum goes upstream for 30" at 13mr  
 $-30 (0.013) =$  -0.390

Distance  $\overline{BC}$  (figure 7)  
 $\frac{.415}{60} = \frac{BC}{30}$  ;  $\overline{BC} = \frac{.45 (30)}{60} =$  -0.207

Distance from the socket line to the working point in figure 7 1.961

The septum sheet angle +13mr

The angle at the back of the septum holder plates + 7mr  
+20mr

GAGE BLOCK CALCULATIONS (refer to figure 2)

The upstream gage point will be 2.875" at 20mr upstream of the end of the electrode

$$2.875 (0.020) = 0.057$$

From the socket line to the inside face of the septum at the upstream end 2.558  
2.615

From the socket line to the edge of the sub-base -0.500

The gage dimension (upstream end) from the edge of the sub-base 2.115 (U<sub>3</sub>)

The septum sheet angle -13mr

The angle at the back of the septum holder plates + 7mr  
- 6mr

The downstream gage point will be 2.125" at 6mr downstream from the end of the electrode

$$2.125 (0.006) = 0.01275 \approx 0.013$$

From the socket line to the inside face of the septum at the downstream end 2.143  
2.156

From the socket line to the edge of the sub-base -0.500

The gage dimension (downstream end) from the edge of the sub-base 1.656 (D<sub>3</sub>)

COPPER SHIELD BLOCK LOCATION

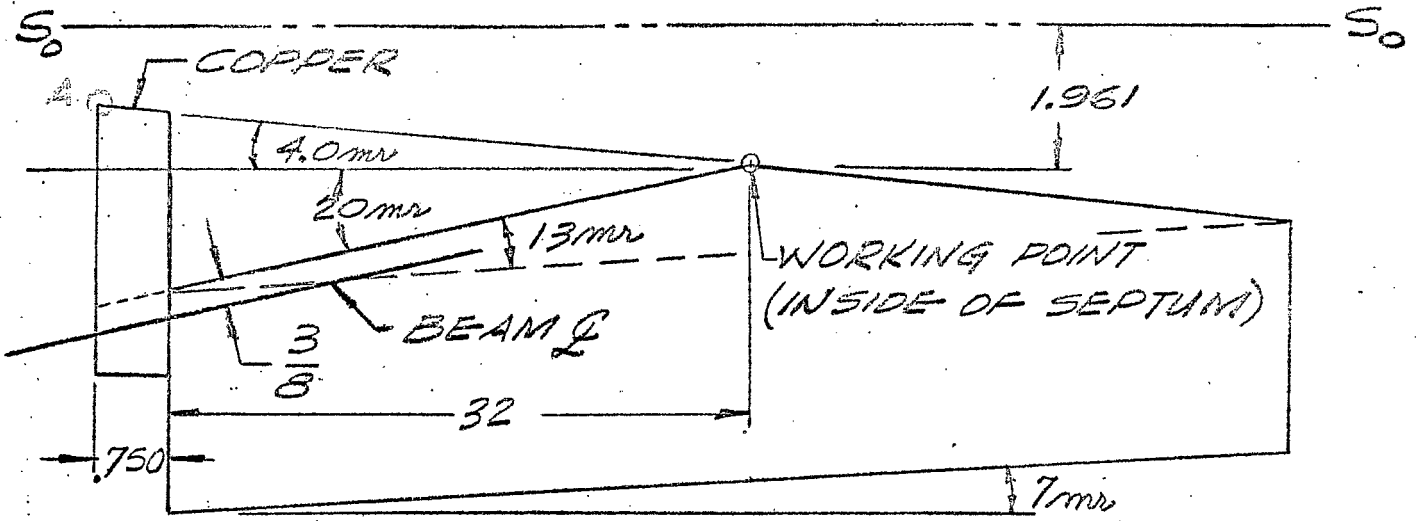


FIGURE 8

From the socket line to the working point	1.961
With a 4mm approach angle at 32.750"	
$-32.750 (0.004) =$	<u>-0.131</u>
	1.830
The septum thickness	<u>-0.015</u>
From the socket line to the leading edge of the copper block, Point "A"	<u>1.815</u>
From the socket line to the edge of the sub-base	<u>-0.500</u>
From the edge of the sub-base to the edge of the copper shield block	<u>1.315</u>

COPPER SHIELD BLOCK DIMENSIONS

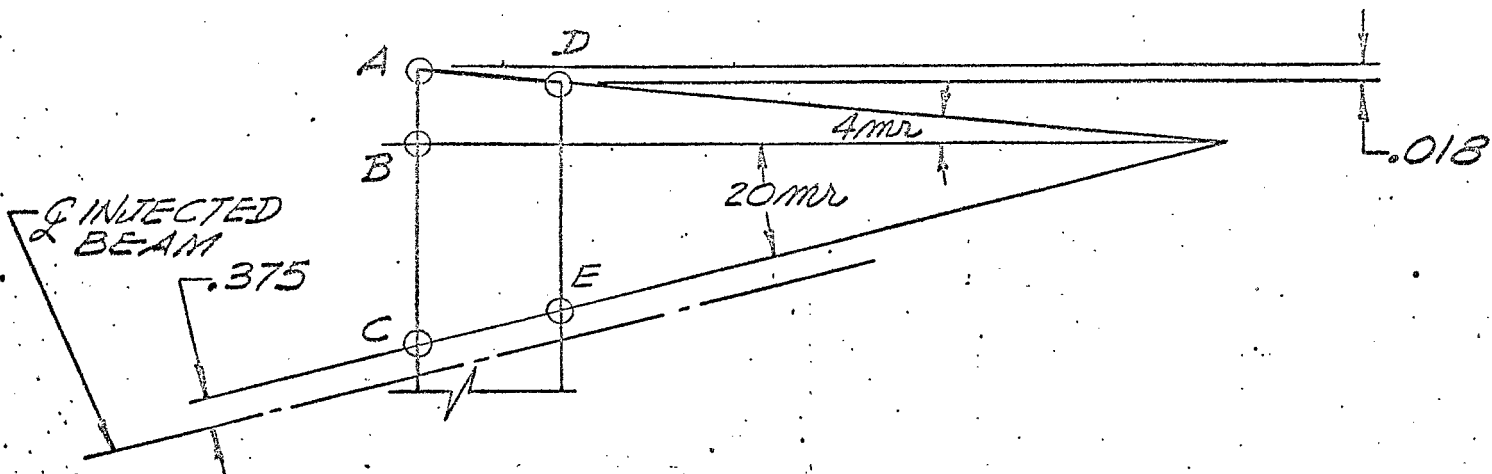


FIGURE 9

BLOCK SLOT POSITION

The vertical distance  $\overline{AB}$

$32.750 (0.004) = 0.131$

The vertical distance  $\overline{BC}$

$32.750 (0.020) = +0.655$

The leading edge of the copper to the inside face of the septum plate 0.786

The septum thickness +0.015

From the edge of the septum to the beam centerline 0.375

From the leading edge of the copper shield block to the slot centerline in the block 1.176

BLOCK LEADING EDGE TAPER

The vertical distance  $\overline{DE}$

$32.000 (0.024) = 0.768$

$0.786$   
 $-0.768$

0.018

UPSTREAM FLAG LOCATION


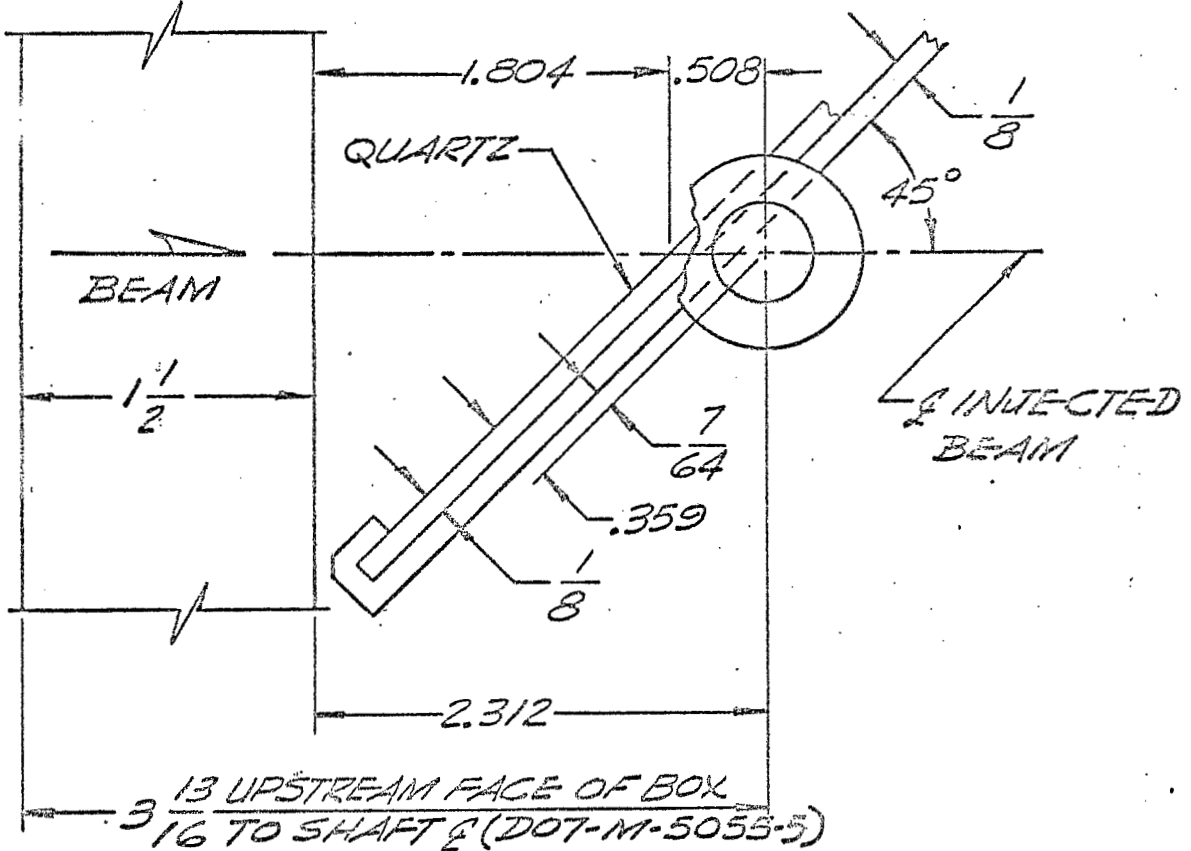


FIGURE 10

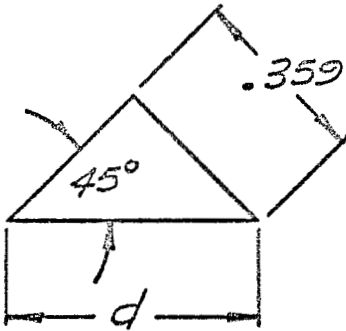

$$(1) \sin 45^\circ = \frac{0.359}{d}$$

$$d = \frac{0.359}{0.707} = 0.5077 \approx 0.508$$

$$(2) \frac{2.312}{1.804} - 0.508 = 1.429$$

From the socket line to the injected beam centerline from figure 6

$$\begin{array}{r} 2.904 \\ +0.161 \\ \hline 3.065 \end{array}$$

From the inside face of the vacuum box to the beam centerline on the quartz

1.804

From the inside face of the vacuum box to the datum line in figure 6

$$\begin{array}{r} -0.375 \\ \hline 1.429 \end{array}$$

The injected beam goes upstream 1.429" at 22mr

1.429 (0.022) =

$$\begin{array}{r} -0.032 \\ \hline 3.033 \end{array}$$

ALTERNATE POSITIONS

There are two secondary, alternate, positions that the inflector could occupy in addition to the primary position that has been described. The first auxilliary position, or middle position, represents a +0.220 outward shift of the working point. The second shift, outer position, is equal to a +0.440 displacement of the working point from the primary position. When the inflector sub-assembly is moved outward the approach angle changes by 2 milliradians per inch of displacement. In addition then, to the outward shift, a clockwise rotation of the inflector sub-assembly is also required. To accomplish these changes of position; 1) additional gage blocks are required, 2) the copper shield block location relative to the socket line and sub-base changes, 3) the flag position changes relative to the socket line. Assuming that the 22 milliradian entrance angle remains the same, the offset to the centerline of the injected beam (figure 6) must also change. As a point of caution, if one or the other of these alternate positions were to be used and evaluated, an outward shift of the entire beam transport from the linac to the inflector may be required, else the beam might scrape the side of the vacuum chamber.

ALTERNATE WORKING POINT POSITIONS

Distance from the socket line to the working point, see figure 7	1.961	
Move inflector sub-assembly out 0.220"	+0.220	
Distance from the socket line to the new working point ( <u>middle position</u> )	<table border="1"><tr><td>2.181</td></tr></table>	2.181
2.181		



Distance from the socket line to the working point, see figure 7 1.961

Move inflector sub-assembly out 0.440" 0.440

Distance from the socket line to the new working point (outer position) 2.401

GAGE BLOCK CALCULATIONS

Middle position:

The gage dimension (upstream end) from the edge of the sub-base, see page 12 2.115

Move inflector out 0.220" +0.220

Since the angle changes 2mr/inch  2.335

$$\frac{2}{1} = \frac{\alpha}{.22} ; \alpha = 0.44 \text{ mr}$$

Upstream gage point is 32,875" upstream of the working point

Rotate the inflector 0.44 mr clockwise about the working point

$$32.875 (0.000444) = 0.0145 \quad -0.014$$

Gage dimension (upstream end) from the edge of the sub-base 2.321 = U<sub>2</sub>

The gage dimension (downstream end) from the edge of the sub-base, see page 12 1.656

Move inflector out 0.220" +0.220

Downstream gage point is 32,125" downstream of the working point  1.876

Rotate the inflector 0.44 mr clockwise about the working point

$$32.125 (0.00044) = 0.0141 \quad +0.014$$

Gage dimension (downstream end) from the edge of the sub-base 1.890 = D<sub>2</sub>

GAGE BLOCK CALCULATIONS

Outer position:

The gage dimension (upstream end) from the edge of the sub-base, see page 12

2.115

Move the inflector out 0.440"

+0.440

Since the angle changes 2mr/inch

2.555

$$\frac{2}{1} = \frac{\beta}{.44} ; \beta = 0.88mr$$

Upstream gage point is 32.875" upstream of the working point

Rotate the inflector 0.88mr clockwise about the working point

$$32.875 (0.00088) = 0.028$$

-0.028

Gage dimension (upstream end) from the edge of the sub-base

$2.527 = U_{1A}$
------------------

The gage dimension (downstream end) from the edge of the sub-base, see page 12

1.656

Move the inflector out 0.440"

+0.440

Downstream gage point is 32.125" downstream of the working point

2.096

Rotate the inflector 0.88mr clockwise about the working point

$$32.125 (0.00088) = 0.028$$

+0.028

Gage dimension (downstream end) from the edge of the sub-base

$2.124 = D_{1A}$
------------------

COPPER SHIELD BLOCK LOCATION

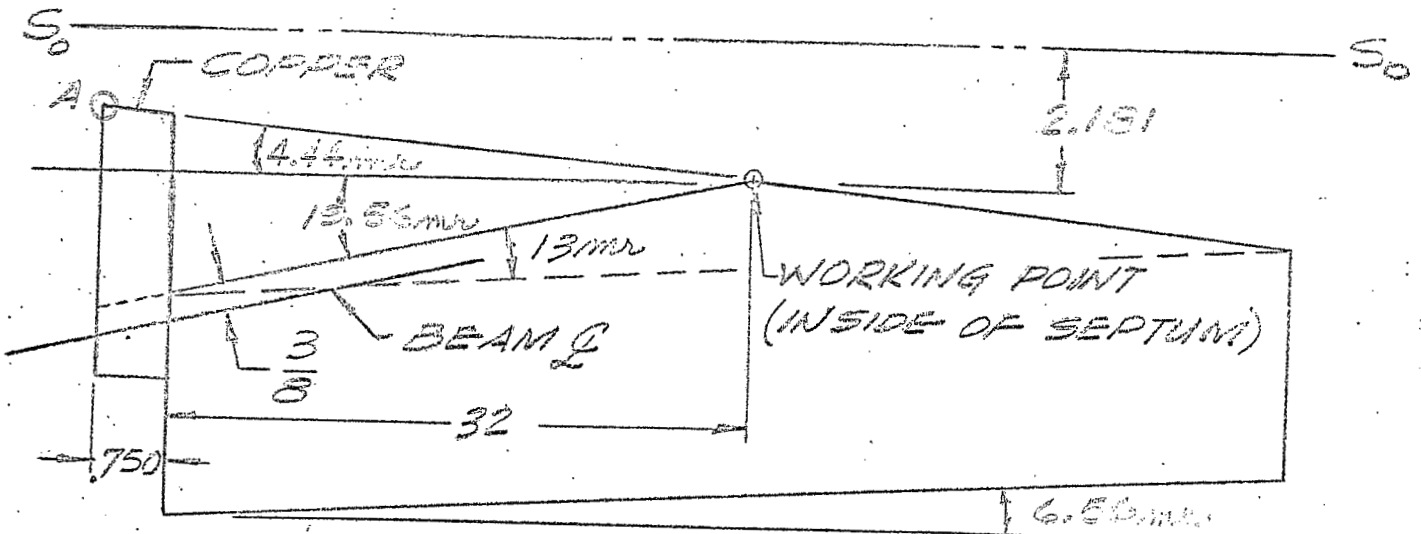


FIGURE 11

MIDDLE POSITION

From the socket line to the working point 1.961

Move the inflector out 0.220" +0.220

Distance from the socket line to the new working point 2.181

The approach angle increases by 0.44mr

With a 4.44mr approach angle at 32.750"

$$32.750 (0.00444) = 0.145$$

The septum thickness +0.015

0.160 -0.160

Socket line to the edge of the copper block, point "A" in figure 11 2.021

Socket line to the edge of the sub-base -0.500

Edge of the sub-base to the edge of the copper block 1.521

COPPER SHIELD BLOCK LOCATION

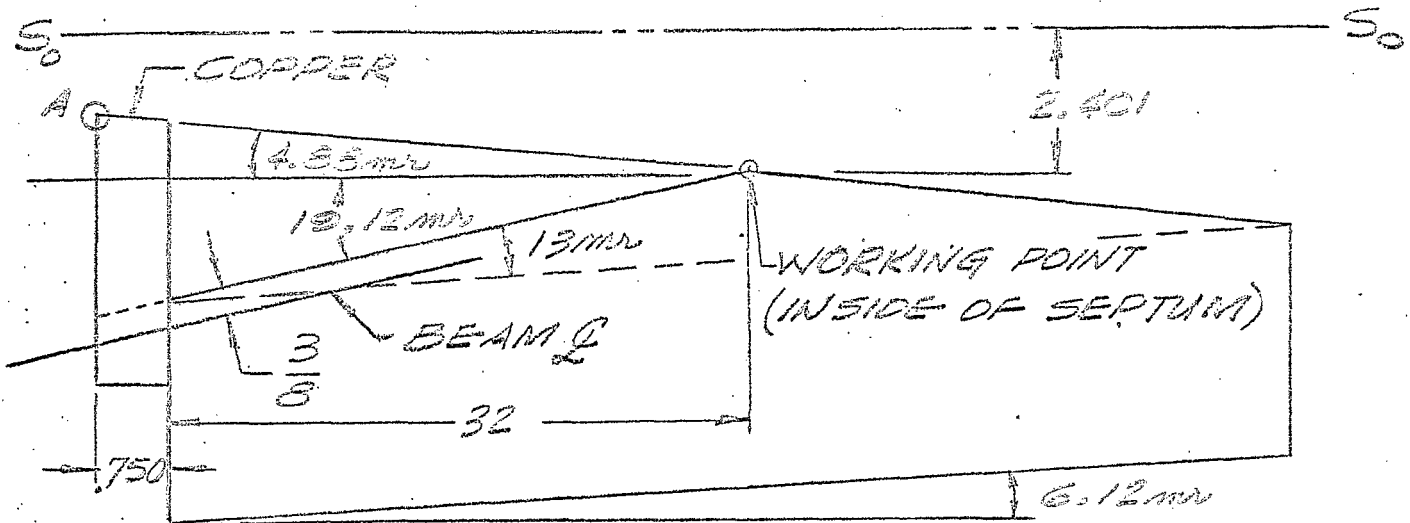


FIGURE 12

OUTER POSITION

From the socket line to the working point		1.961
Move the inflector out 0.44"		+0.440
		<hr/>
Distance from the socket line to the new working point		2.401
The approach angle increases by 0.88mr		
With a 4.88mr approach angle at 32.750"		
$32.750 (0.00488) = 0.160$		
The septum thickness	+0.015	
	<hr/>	
	0.175	-0.175
		<hr/>
Socket line to the edge of the copper block, point "A" in figure 12		<span style="border: 1px solid black; padding: 2px;">2.226</span>
Socket line to the edge of the sub-base		-0.500
		<hr/>
Edge of the sub-base to the edge of the copper block		<span style="border: 1px solid black; padding: 2px;">1.726</span>

OFFSET TO THE INJECTION LINE

Middle position:

Upstream gage block dimensions, see page 17	2.321	
Socket line to the edge of the sub-base	<u>+0.500</u>	
	2.821	
Move downstream 2.875" at 19.56mr	<u>-0.056</u>	
Socket line to the inside face of the septum at the upstream end of the electrode	2.765	
Centerline of the 1/2" dia. beam will enter the inflexor 3/8" from the inside of the septum	<u>+0.375</u>	
	3.140	
Offset 6" downstream at 22mr		
6.000 (0.022) =	<u>+0.132</u>	
y <sub>1</sub> from page 9 = 0.035	3.272	
y <sub>2</sub> from page 9 = <u>+0.126</u>		
0.161	<u>-0.161</u>	
Offset to the injection line (middle position)	<table border="1"><tr><td>3.111</td></tr></table>	3.111
3.111		

Outer position:

Upstream gage block dimension, see page 18	2.527	
Socket line to the edge of the sub-base	<u>+0.500</u>	
	3.027	
Move downstream 2.875" at 19.12mr	<u>-0.055</u>	
Socket line to the inside face of the septum at the upstream end of the electrode	2.972	
Centerline of the 1/2" dia. beam will enter the inflexor 3/8" from the inside of the septum	<u>+0.375</u>	
	3.347	
Offset 6" downstream at 22mr	<u>+0.132</u>	
	3.479	
y <sub>1</sub> + y <sub>2</sub> = 0.161	<u>-0.161</u>	
Offset to the injection line (outside position)	<table border="1"><tr><td>3.318</td></tr></table>	3.318
3.318		

ALTERNATE FLAG LOCATIONS

Middle position:

Offset to the injection line, see page 21 3.111

$y_1 + y_2 = 0.161$  from page 9 +0.161  
3.272

Move 1.429" upstream at 22mr, see page 15

1.429 (0.022) = -0.032

From the socket line to the flag centerline 3.240

Outer position:

Offset to the injection line, see page 21 3.318

$y_1 + y_2 = 0.161$  from page 9 +0.161  
3.479

Move 1.429" upstream at 22mr, see page 15

1.429 (0.022) = -0.032

From the socket line to the flag centerline 3.447

SUMMARY OF DATA

Location	Socket line to the Working Point	Gage Block Dimensions	Gage Block Symbols *	Socket line to edge of the copper block	Socket line to the Quartz Flag
Primary	1.961	2.115	U <sub>3</sub>	1.815	3.033
		1.656	D <sub>3</sub>		
Middle	2.181	2.321	U <sub>2</sub>	2.021	3.240
		1.890	D <sub>2</sub>		
Outer	2.401	2.527	U <sub>1A</sub>	2.226	3.447
		2.124	D <sub>1A</sub>		

\* "U" denotes upstream and "D" denotes downstream

Distr: Department Administration  
Mechanical Engineers  
Operations Coordinators  
J. Grisoli  
J. Herrera  
E. Raka