



BNL-104509-2014-TECH

AGS/AD/Tech Note No. 76;BNL-104509-2014-IR

VACUUM SYSTEM FOR THE H-10 EJECTOR MAGNET ASSEMBLY

J. C. Schuchman

March 1970

Collider Accelerator Department
Brookhaven National Laboratory

U.S. Department of Energy

USDOE Office of Science (SC)

Notice: This technical note has been authored by employees of Brookhaven Science Associates, LLC under Contract No.AT(30-1)-16 with the U.S. Department of Energy. The publisher by accepting the technical note for publication acknowledges that the United States Government retains a non-exclusive, paid-up, irrevocable, world-wide license to publish or reproduce the published form of this technical note, or allow others to do so, for United States Government purposes.

DISCLAIMER

This report was prepared as an account of work sponsored by an agency of the United States Government. Neither the United States Government nor any agency thereof, nor any of their employees, nor any of their contractors, subcontractors, or their employees, makes any warranty, express or implied, or assumes any legal liability or responsibility for the accuracy, completeness, or any third party's use or the results of such use of any information, apparatus, product, or process disclosed, or represents that its use would not infringe privately owned rights. Reference herein to any specific commercial product, process, or service by trade name, trademark, manufacturer, or otherwise, does not necessarily constitute or imply its endorsement, recommendation, or favoring by the United States Government or any agency thereof or its contractors or subcontractors. The views and opinions of authors expressed herein do not necessarily state or reflect those of the United States Government or any agency thereof.

Accelerator Department
BROOKHAVEN NATIONAL LABORATORY
Associated Universities, Inc.
Upton, New York

AGS DIVISION TECHNICAL NOTE

No. 76

J.C. Schuchman
March 16, 1970

VACUUM SYSTEM FOR THE H-10 EJECTOR MAGNET ASSEMBLY

Summary

This note describes the technique for pumping the new H-10 ejector magnet assembly.

The technique is to condition the magnet and box assembly prior to its installation in the ring. The conditioning is a mild bakeout of the magnet assembly while under vacuum. The bakeout will be at 250°F for 24 hours. The vacuum system proper will consist of four small ion pumps, (150-200 μ /sec) connected directly to the box without valves. After conditioning, the assembly will remain under vacuum until it is scheduled for installation in the ring. At that time, it will be vented with dry nitrogen and the entire assembly, box, magnet, pumps, etc., will be installed as a single unit. The operating pressure is calculated as below the design pressure of 1×10^{-6} torr.

Discussion

As with any vacuum system, the most difficult quantity to estimate or measure is the gas load; that is, the outgassing rates of the various components which make up the assembly. Therefore, calculations are based on the performance of F10 as well as outgassing rates measured on the "dry-stacked" and the "epoxy" magnet assemblies. The "dry-stacked" magnet refers

to the magnet assembly which used an oxide film to insulate the laminations while the "epoxy" magnet used epoxy in addition to an oxide film between laminations.

Starting with the lowest recorded operating pressure at the F-10 box of 1.7×10^{-6} torr and assuming a total pumping speed at the F-10 box of 490 ℓ /sec, the gas load pumped is $Q = PS = (1.7 \times 10^{-6} \text{ torr}) (490 \text{ } \ell/\text{sec}) = 8.3 \times 10^{-4} \text{ T}\ell/\text{sec}$. This is for an epoxy magnet. Since a dry-stacked magnet will be used at H-10, this number must be adjusted to suit. Relative outgassing rate measurements made on sample magnets show that the dry-stacked magnet outgasses about 2.4 times more than the epoxy magnet, see Fig. 1. Therefore, the total gas load anticipated for H-10 is

$$(2.4) (8.3 \times 10^{-4}) = 20 \times 10^{-4} \text{ T}\ell/\text{sec}.$$

If an operating pressure of 1×10^{-6} torr is desired then the required pumping speed is $\frac{Q}{P} = \frac{20 \times 10^{-4}}{1 \times 10^{-6}} = 2000 \text{ } \ell/\text{sec}$.

One means of obtaining this speed is to use two 1500 ℓ /sec pumps which would have an effective speed of 2000 ℓ /sec. Another solution, and the one taken here, is to reduce the gas load, and hence the required pumping speed, by baking the entire magnet assembly. Our tests have shown that the outgassing rate of the dry-stacked magnet can be reduced 75% by baking the magnet at 200^oF for 24 hours, see Fig. 2. Applying this reduction to the H10 gas load, $(20 \times 10^{-4} \text{ T}\ell/\text{sec}) (25\%) = 5 \times 10^{-4} \text{ T}\ell/\text{sec}$. If four small pumps (200 ℓ /sec) are now used on the box, a total of 780 ℓ /sec is available. Therefore, a base pressure of a baked out magnet assembly would be

$$\frac{5 \times 10^{-4} \text{ T}\ell/\text{sec}}{780 \text{ } \ell/\text{sec}} = 6.4 \times 10^{-7} \text{ torr}.$$

If one pump was inoperative the effective speed would be reduced to 590 l/sec and the pressure would be

$$\frac{5 \times 10^{-4}}{590} = 8.5 \times 10^{-7} \text{ torr.}$$

It is important to point out that all of the above calculations are based on data measured after a couple of days of pumping. Figure 3 shows a pump down curve for the AGS half superperiod mock-up,¹ which may be considered as typical for the converted AGS. It shows a nominal operating pressure in the 10^{-7} torr area. I would estimate that the pressure in a typical 10 ft box, such as we are discussing, will follow the AGS pump down curve, but will be higher by a factor of about five. This would indicate that after five hours of pumping the 10 ft box would be below 5×10^{-5} torr which is the high pressure cut off point for the AGS.

References


1. T. Carides and J.G. Cottingham, "Wet vs Dry Venting of a Vacuum Chamber," AGSCD Technical Note No. 81, June 1967.

Distr: Department Administration
AGS Division Staff

$g = \text{TR/sec cm}^2 \rightarrow$


Fig. 1

TIME HOURS \rightarrow

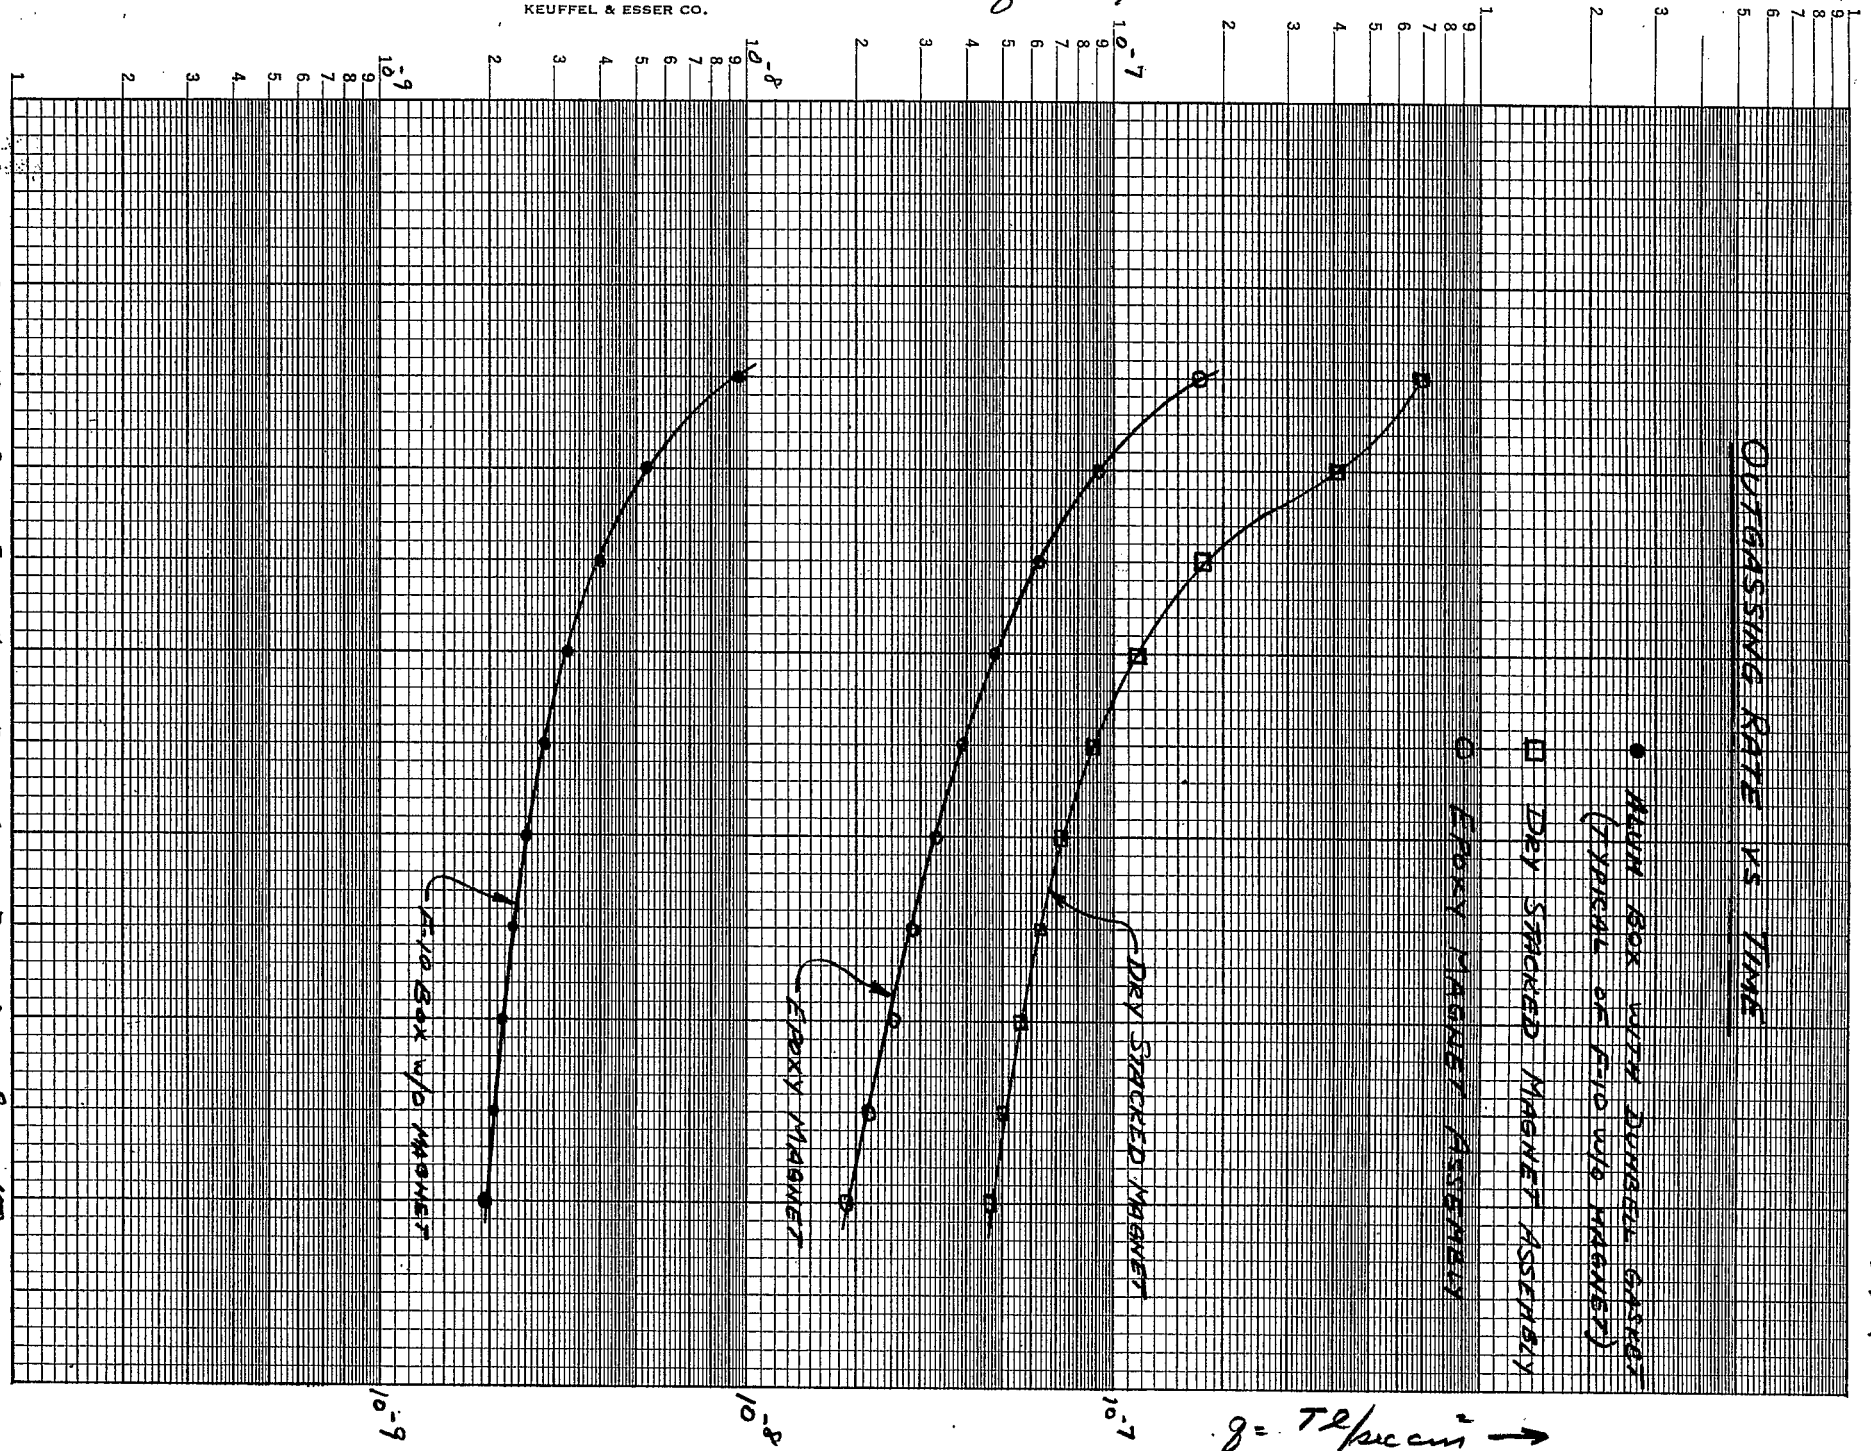

$g = \text{TR/sec cm}^2 \rightarrow$

DRY STACKED MAGNET

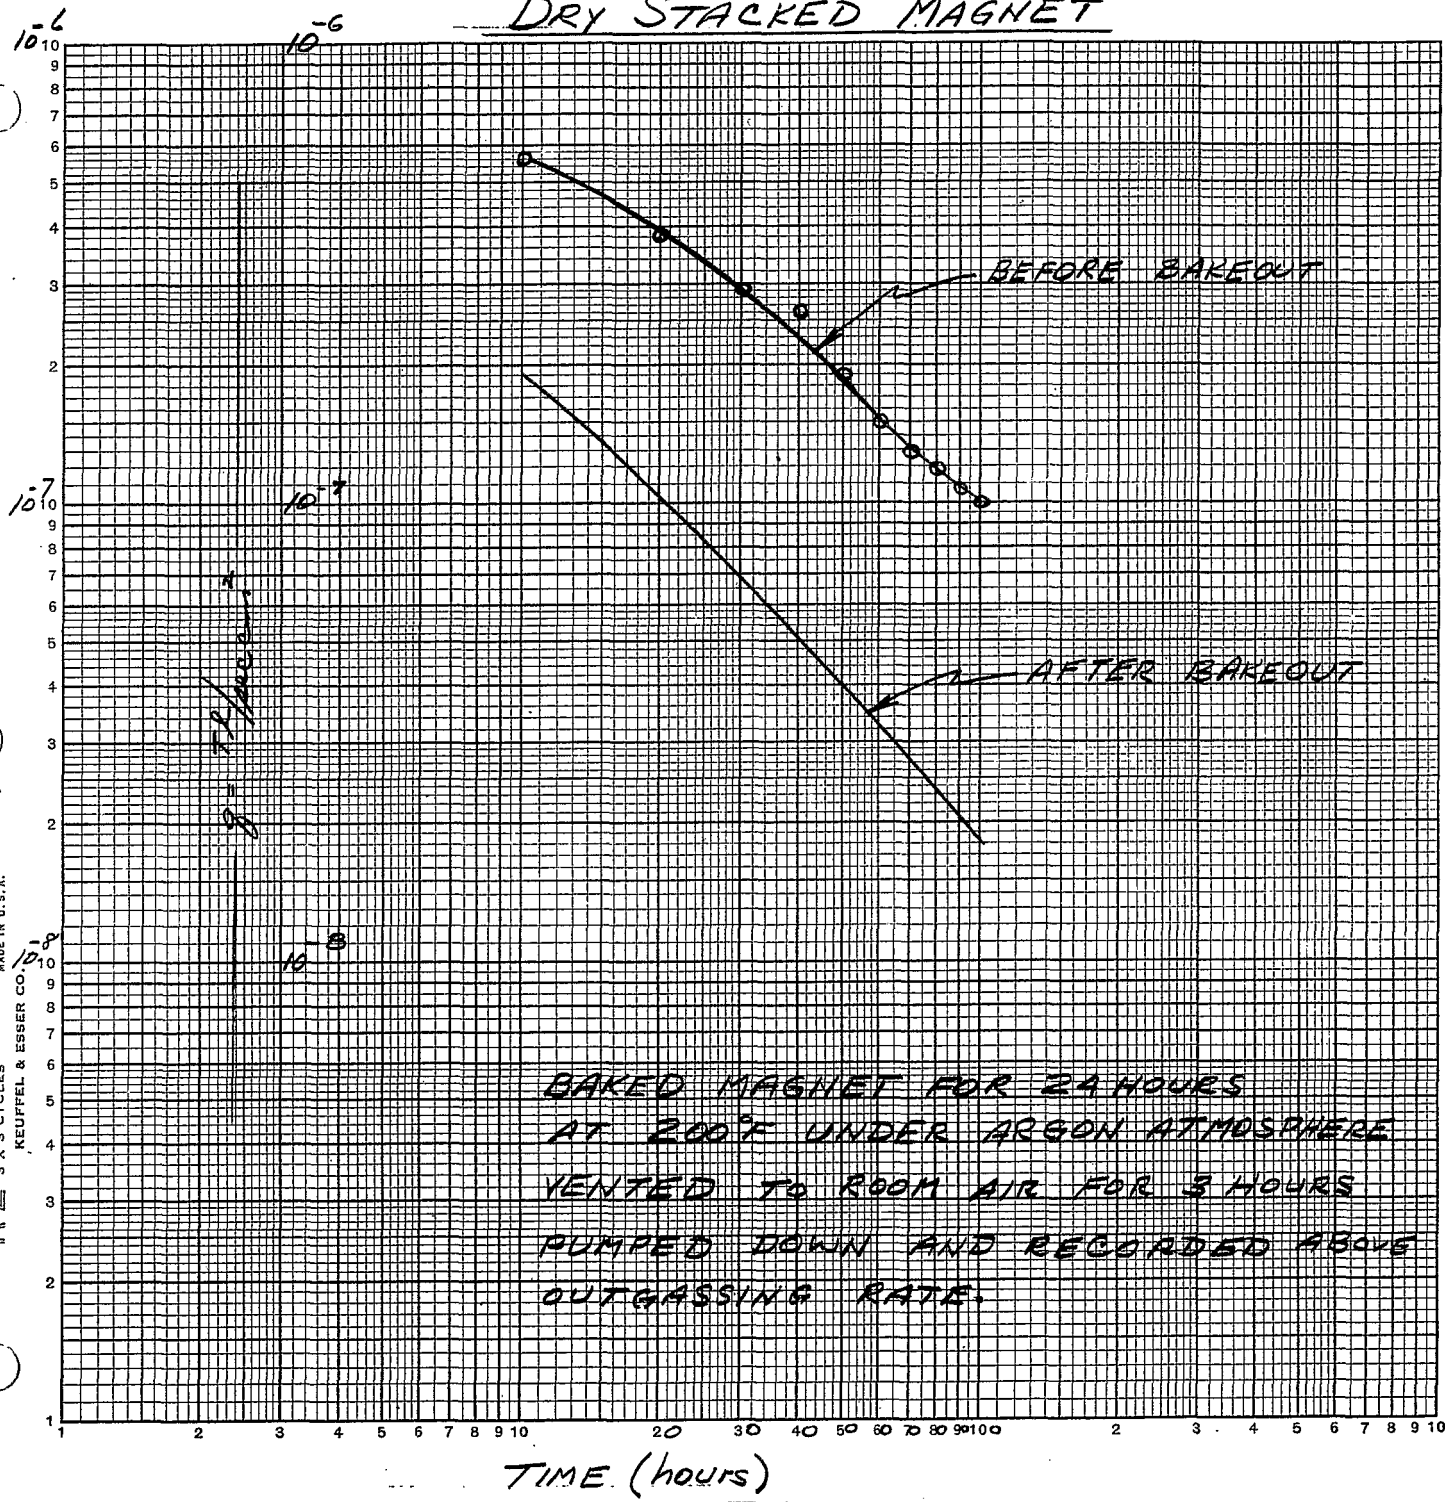

46 7400
MADE IN U.S.A.
LOGARITHMIC
3 X 3 CYCLES
KEUFFEL & ESSER CO.


Fig 2 OUTGASSING RATE OF DRY-STACKED
MAGNET BEFORE AND AFTER BAKE

OUTGASSING RATE VS TIME

- ALUM BOX WITH DUMBBELL GASKET (TYPICAL OF F10 W/O MAGNET)
- DRY STACKED MAGNET ASSEMBLY
- EPOXY MAGNET ASSEMBLY

g TPR/area cm²

g TPR/cm²

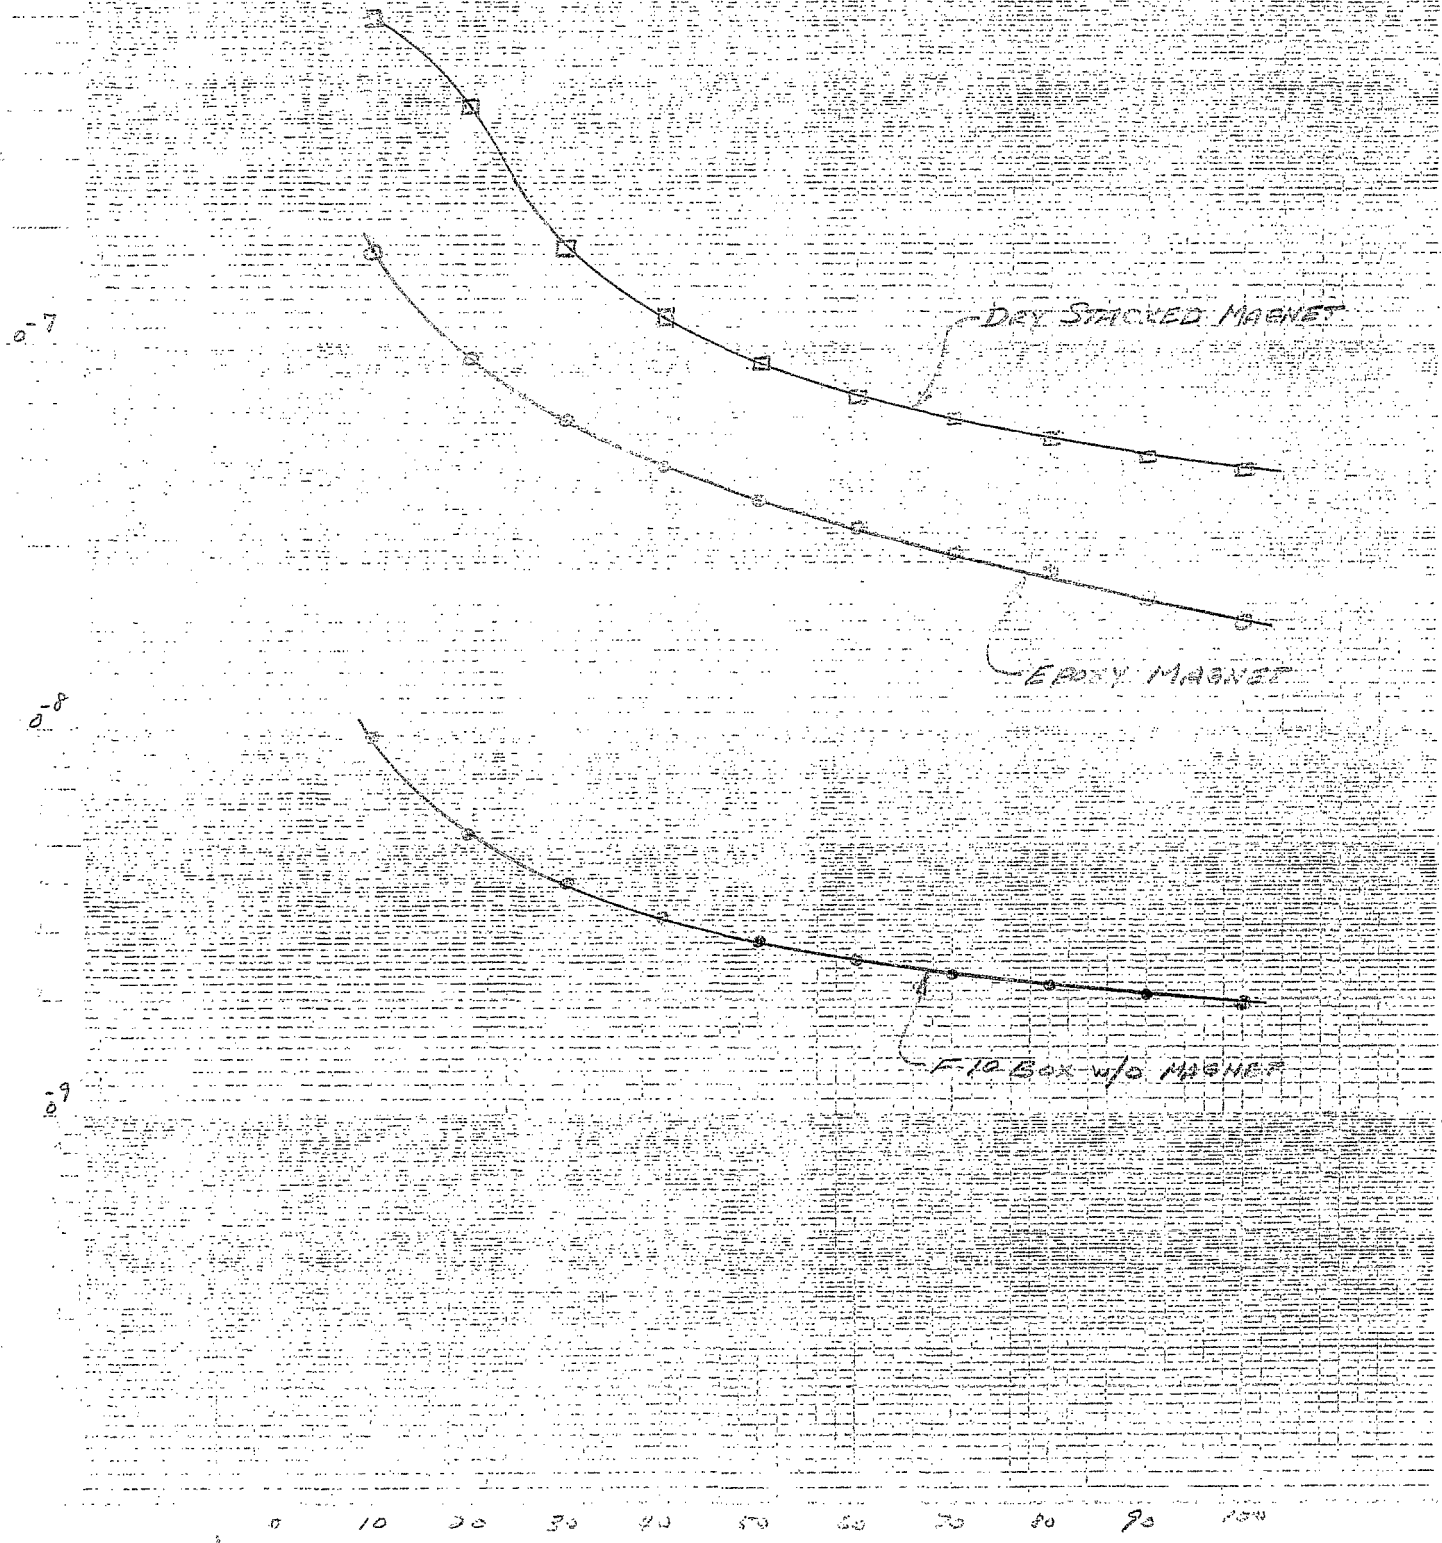


10⁻⁷

10⁻⁸

10⁻⁹

1947
JUL

DRY STACKED MAGNET

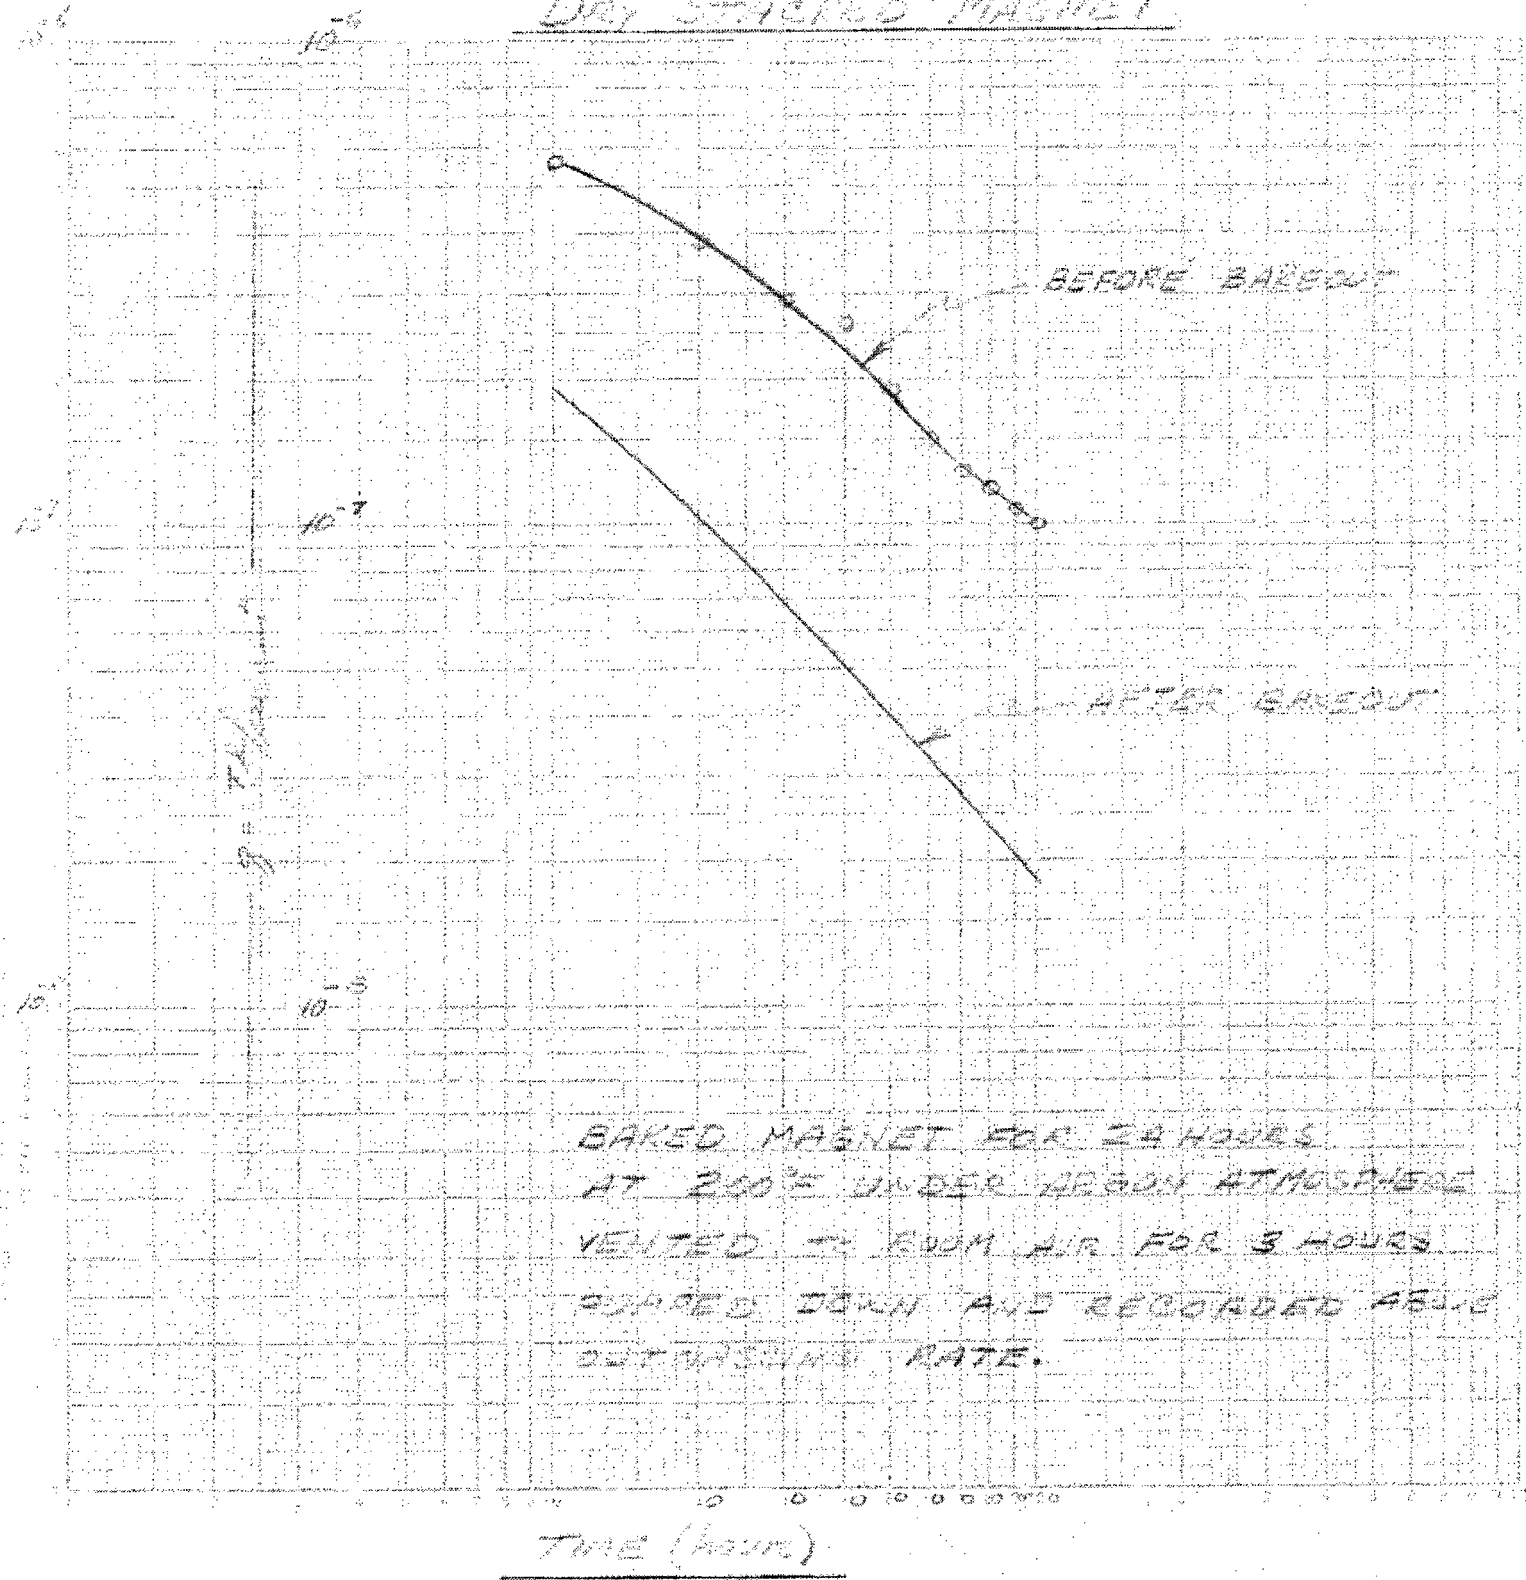

BAKED MAGNET FOR 24 HOURS
 AT 200°C UNDER ROOM ATMOSPHERE
 VENTED TO ROOM AIR FOR 3 HOURS
 REWOUND DOWN AND RECORDED AS USUAL
 OBTAINING RATE.

TIME (hour)

Fig 2 DISCHARGING RATE OF DRY-STACKED
 MAGNET BEFORE AND AFTER BAKING

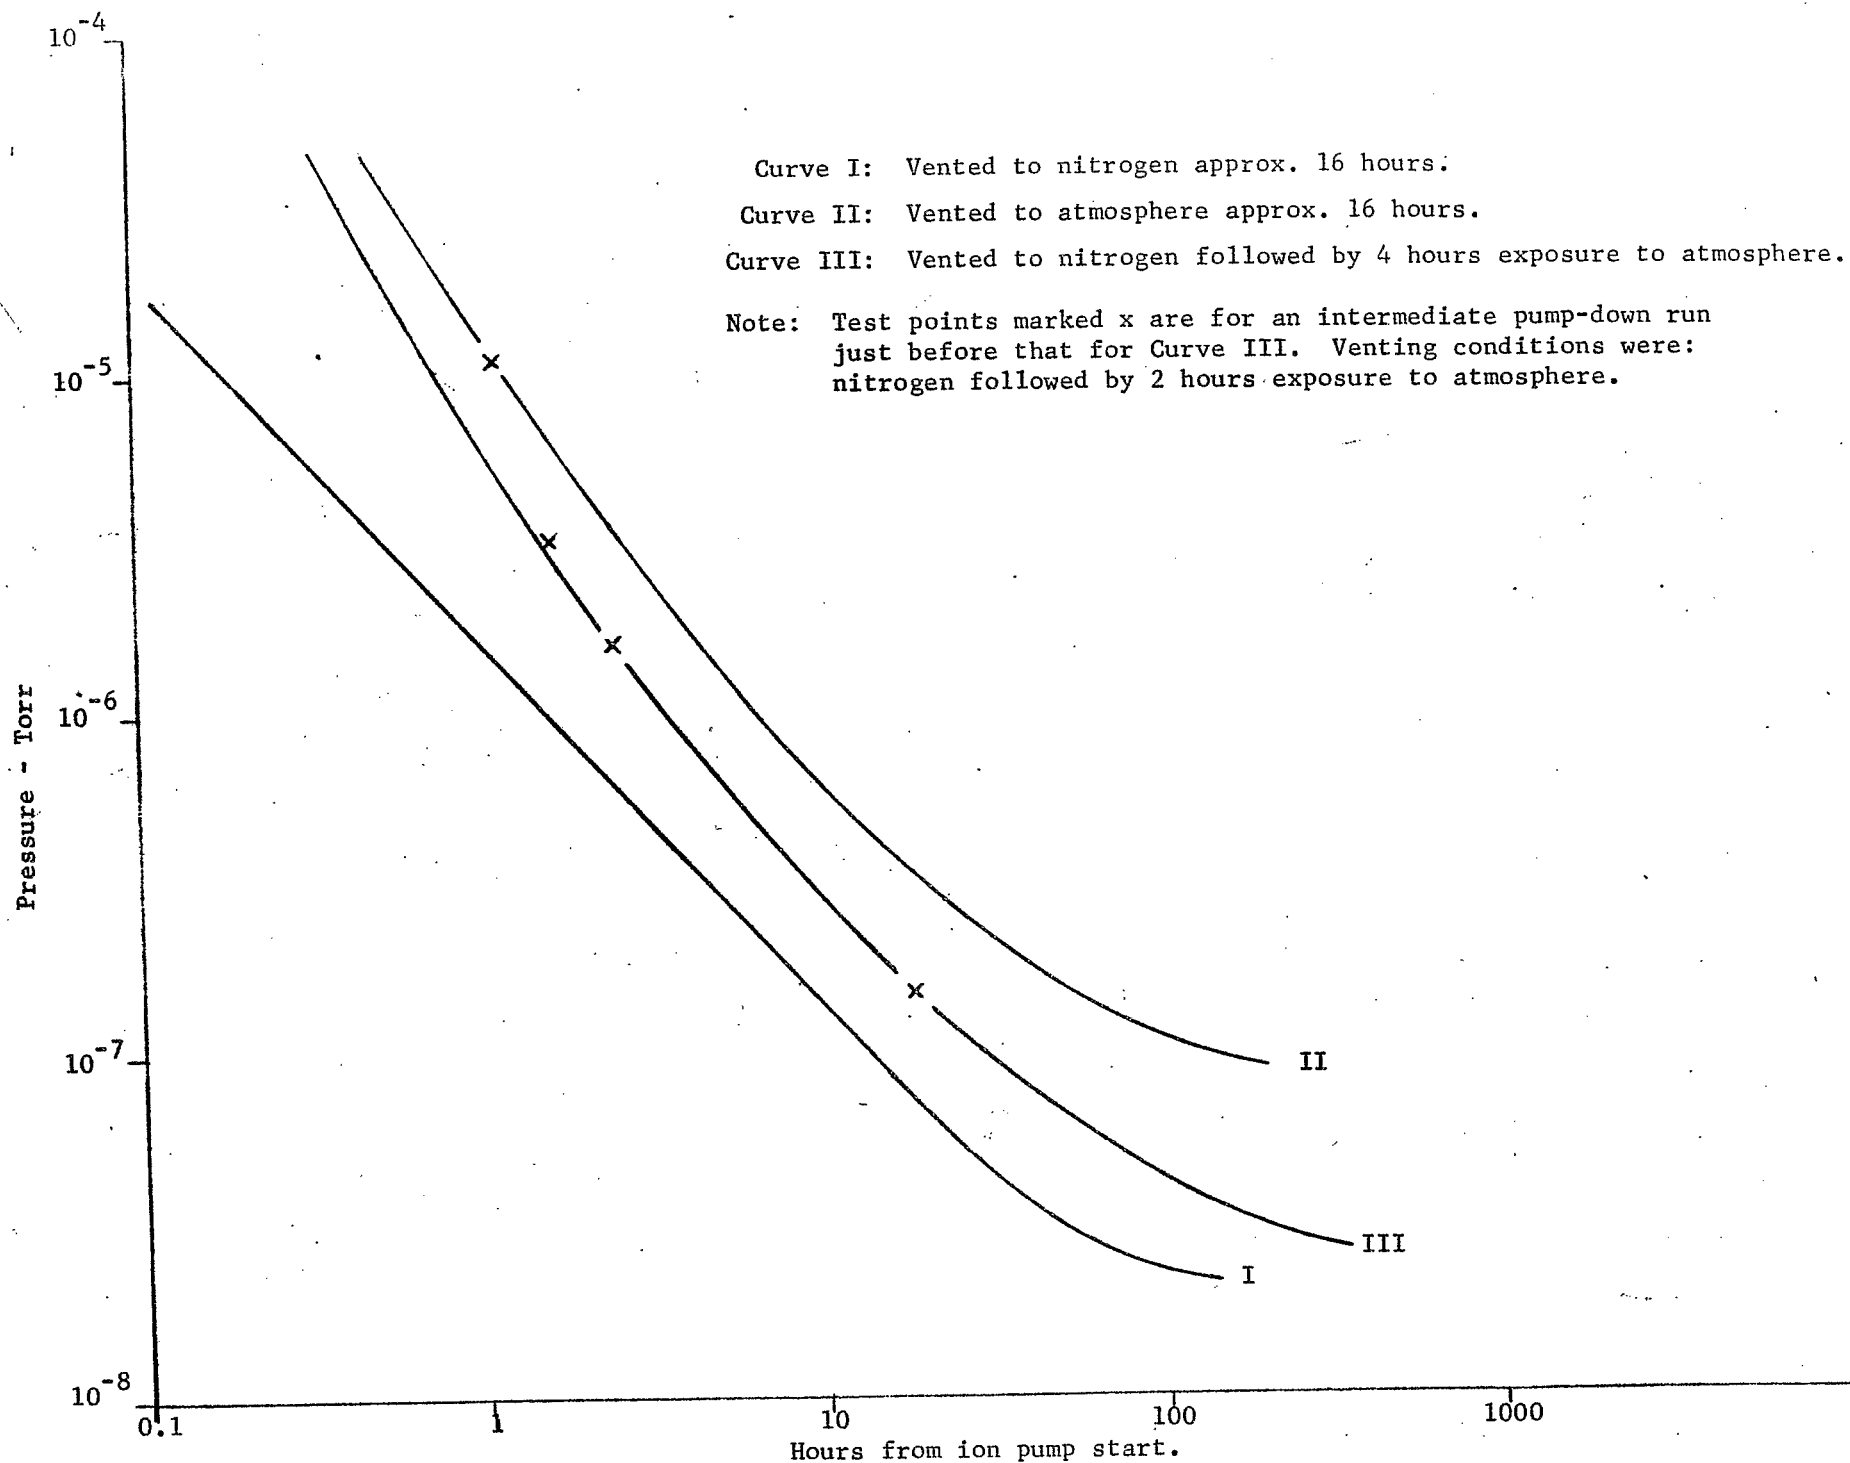


Fig. 3. Pump-down characteristics for various venting conditions.