



BNL-104558-2014-TECH

AGS/AD/Tech Note No. 129;BNL-104558-2014-IR

# CONSTRUCTION OF LOWER INTENSITY PRIMARY PROTON BEAM

Y. Y. Lee

January 1977

Collider Accelerator Department  
**Brookhaven National Laboratory**

**U.S. Department of Energy**

USDOE Office of Science (SC)

Notice: This technical note has been authored by employees of Brookhaven Science Associates, LLC under Contract No.EY-76-C-02-0016 with the U.S. Department of Energy. The publisher by accepting the technical note for publication acknowledges that the United States Government retains a non-exclusive, paid-up, irrevocable, world-wide license to publish or reproduce the published form of this technical note, or allow others to do so, for United States Government purposes.

## **DISCLAIMER**

This report was prepared as an account of work sponsored by an agency of the United States Government. Neither the United States Government nor any agency thereof, nor any of their employees, nor any of their contractors, subcontractors, or their employees, makes any warranty, express or implied, or assumes any legal liability or responsibility for the accuracy, completeness, or any third party's use or the results of such use of any information, apparatus, product, or process disclosed, or represents that its use would not infringe privately owned rights. Reference herein to any specific commercial product, process, or service by trade name, trademark, manufacturer, or otherwise, does not necessarily constitute or imply its endorsement, recommendation, or favoring by the United States Government or any agency thereof or its contractors or subcontractors. The views and opinions of authors expressed herein do not necessarily state or reflect those of the United States Government or any agency thereof.

Accelerator Department  
BROOKHAVEN NATIONAL LABORATORY  
Associated Universities, Inc.  
Upton, New York

AGS DIVISION TECHNICAL NOTE

No. 129

CONSTRUCTION OF LOWER INTENSITY PRIMARY PROTON BEAM

Y.Y. Lee  
January 12, 1977

In recent years, there has been considerable interest for the experiments utilizing slowly extracted primary proton beams. The range of intensities interested were between  $10^6$  to several times  $10^{12}$  depending on the experiment. There was proton beam of primary energy from the "old A" station intensity about  $10^6$  protons per pulse. The method used was to utilize the diffracted protons from the "old A" target. The intensity range was less than  $10^7$  protons. Another example of the primary proton beam was to finely split the slow extracted beam to the new A station for Experiment 598. The lowest intensity one can run stably was a few times  $10^{10}$  protons pulse. There was, however, a large gap between the two methods. It should be noted also that there is no easy way to switch between the two methods. In this context, it is very desirable to have a beam designed to have a continuous intensity range of  $10^6$  to  $10^{12}$  protons per pulse.

We constructed the primary proton beam covering a range of this region from the new A station to the secondary branch line to the A3 branch of the HEUB. The beam was designed primarily for Experiment 676 which measures prompt muons. The experimental requirement for the incident proton is to have an intensity of less than  $10^6$  to more than  $10^{12}$  protons depends on the experimental program.

Figure 1 shows the plan view of the floor layout of the beam. The slow ejected beam from the F10 extractor magnet is split by the thin magnetic septum to A and BC stations. The details of the optics of the primary proton beam can be referred to other publications.<sup>1</sup> The experience shows one can stably run the A-line with the intensity down to a few times  $10^{10}$  protons per

pulse. In order to get the intensity of  $10^6$  protons per pulse we should limit the phase space acceptance of about  $10^{-4}$  of the original phase space. We placed the collimator of 1 m brass. The collimator has three fixed holes, and the smallest was 1/16" X 1/16" square hole chosen by the beam stability and accuracy of alignment. The next two holes are ten and one hundred times of the area of the smallest hole. The intensity lower than  $10^7$  proton per pulse was adjusted by setting the primary beam to the edge of the phase space, in other words, set the hole around the halo area. In order to use the position along the phase space ellipse to control the intensity of the beam, the following condition is desirable. When the main bending and pitching magnet change the value, focusing condition should be set such that the position of the beam moves along the major axis of the phase ellipse at the collimator. The computer program was used to find such a solution. The solution was to turn both the focusing quadrupoles upstream of "A" target off. The small trimming was necessary with AQ4AB which is located downstream of the first bender.

Figure 2 shows the phase space ellipse at the "A" target station and at the Experiment 676 target. The cross hatched area represents the area of the small collimator hole.


About  $10^{-3}$  of the original proton survives the absorption in one meter of brass collimator. They can be cleaned up in subsequent collimators. The energy loss through the one meter collimator is about 1.3 GeV and corresponding to  $\sim 4.5\%$  at A.G.S. energy. The difference of momentum is just enough to be cleaned up by the optical system. Since the beam A3 has two large bends  $4.8^\circ$  and  $10^\circ$ , the discrimination against different energy is quite easy. Since we are dealing with the large amount of unwanted off momentum particles, momentum recombination was not done for the downstream of the intensity defining collimator.

The operational experience for this beam has been quite successful and satisfactory for all phases of the Experiment 676.


#### Reference

1. See for example, AGS Technical Report 1126.

Distr.: Accel. Dept. S&P

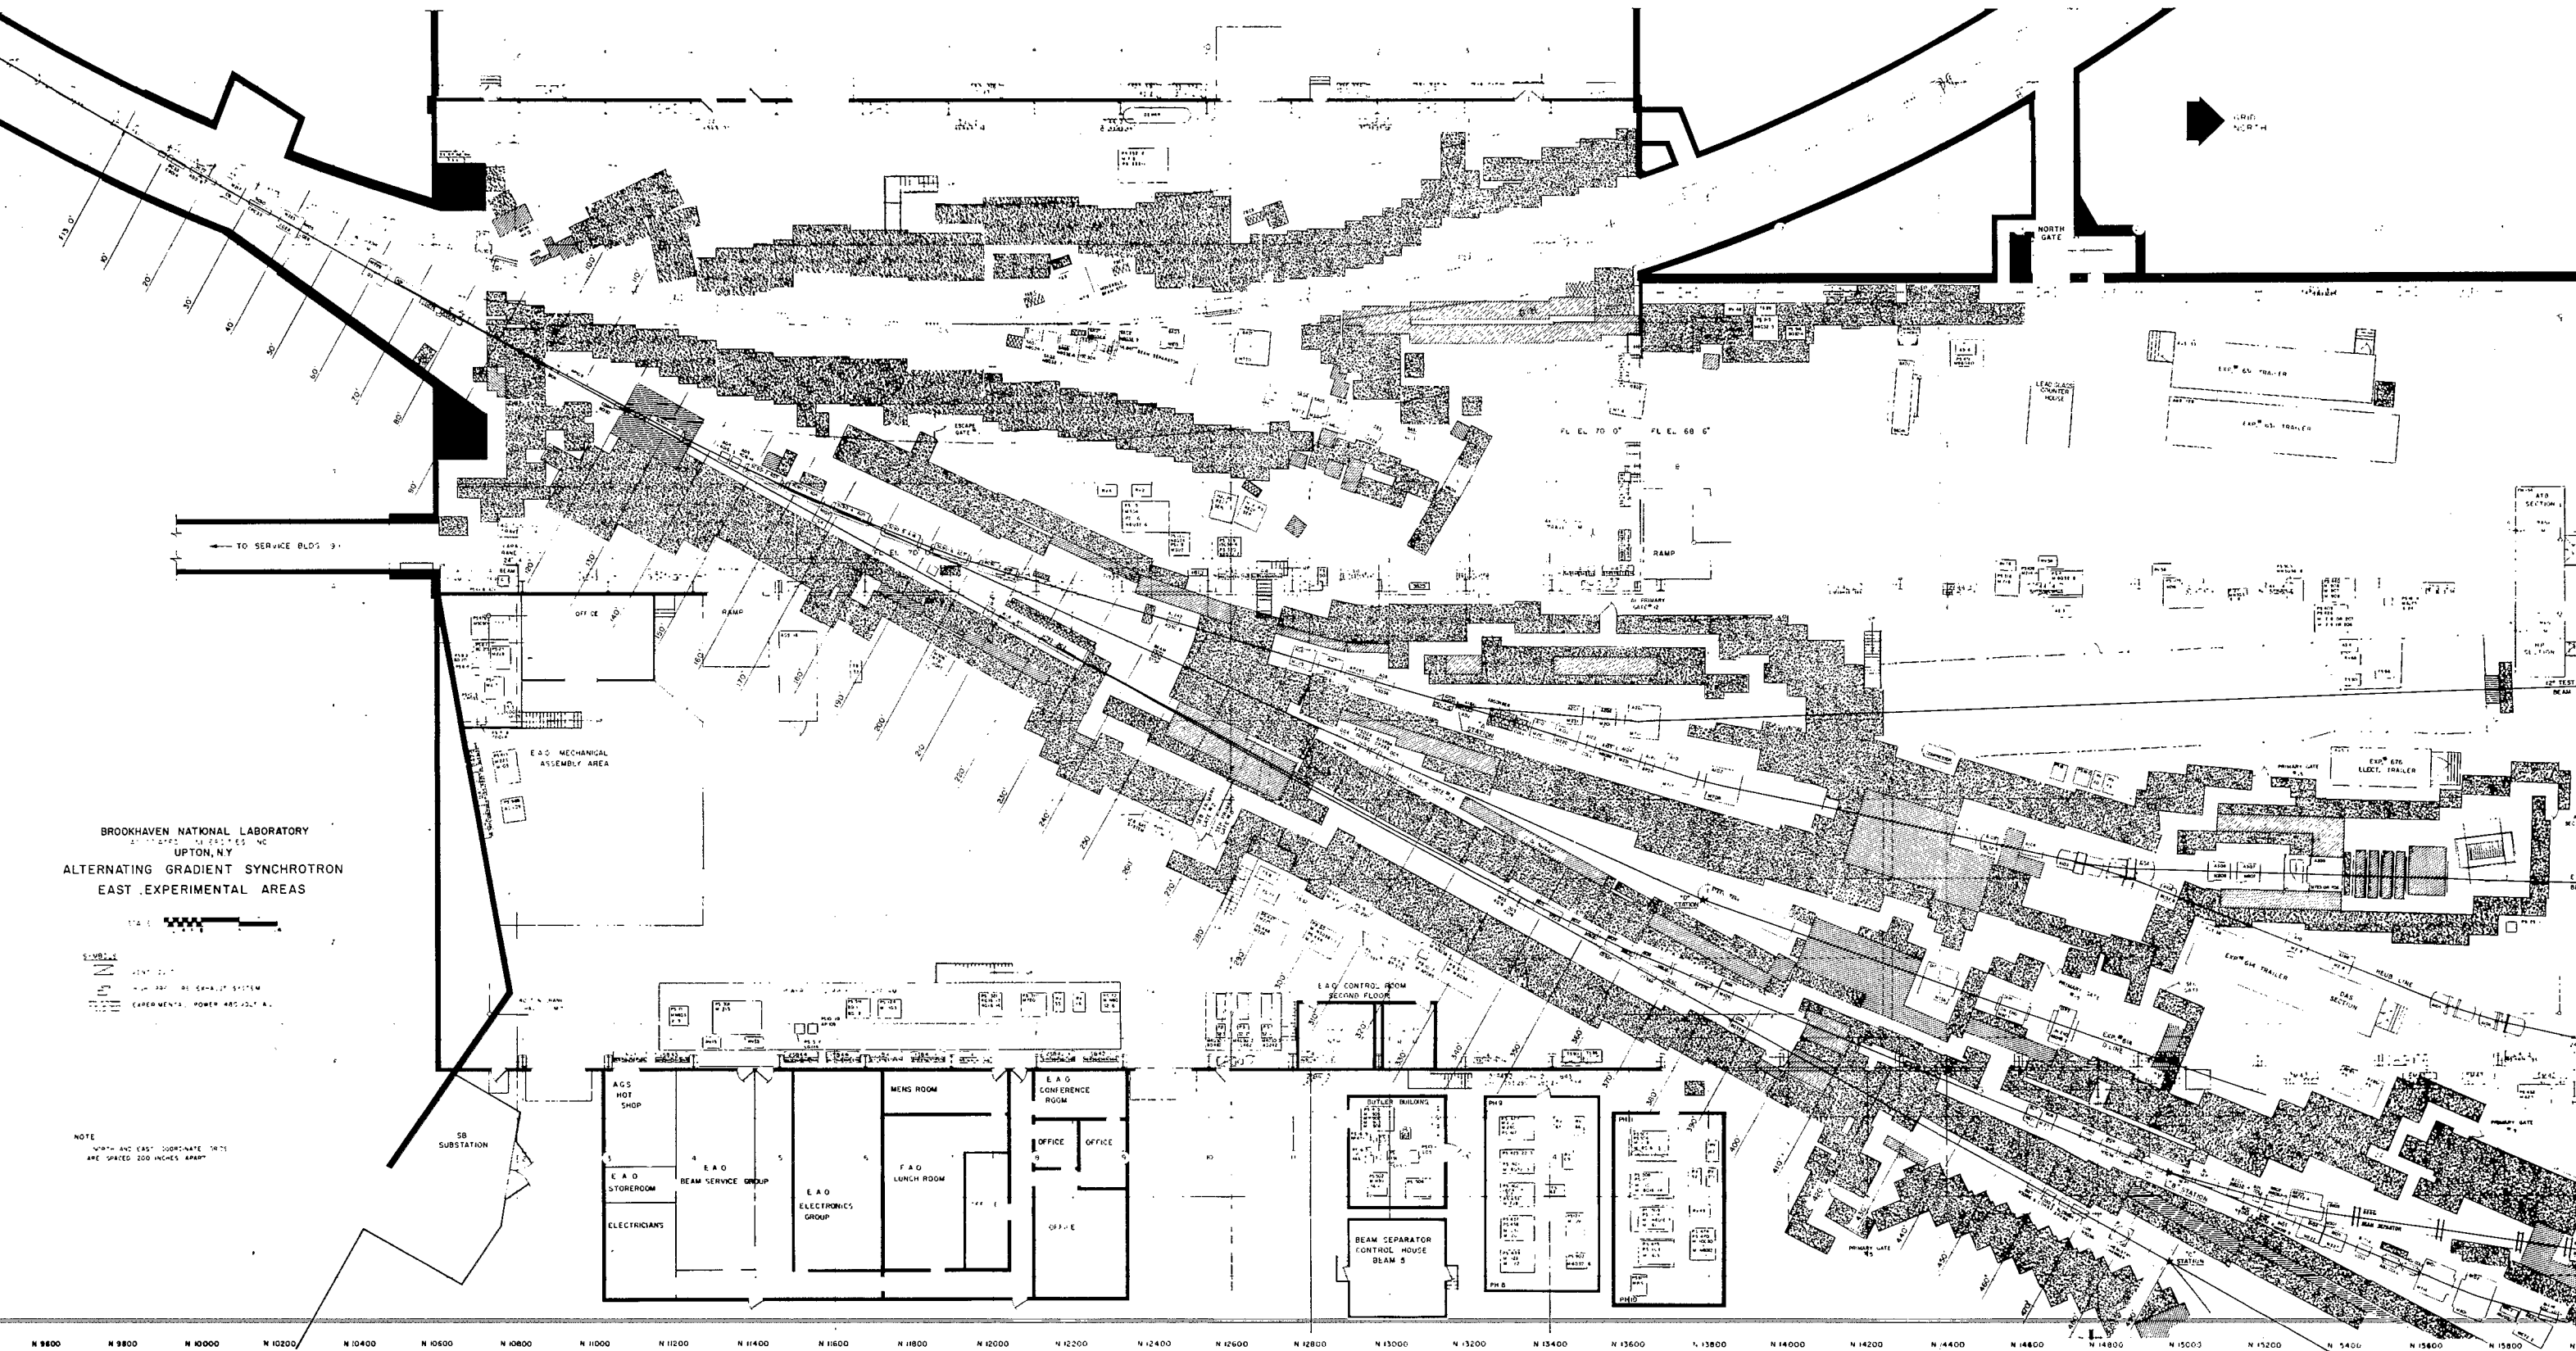

BROOKHAVEN NATIONAL LABORATORY  
 UPTON, NY  
 ALTERNATING GRADIENT SYNCHROTRON  
 EAST EXPERIMENTAL AREAS




SYMBOLS  
 (various symbols for doors, windows, etc.)  
 (various symbols for equipment, etc.)


NOTE  
 NORTH AND EAST COORDINATE VALUES  
 ARE SPACED 200 INCHES APART

N 9800 N 9800 N 10000 N 10200 N 10400 N 10600 N 10800 N 11000 N 11200 N 11400 N 11600 N 11800 N 12000 N 12200 N 12400 N 12600 N 12800 N 13000 N 13200 N 13400 N 13600 N 13800 N 14000 N 14200 N 14400 N 14600 N 14800 N 15000 N 15200 N 15400 N 15600 N 15800

FIG 1

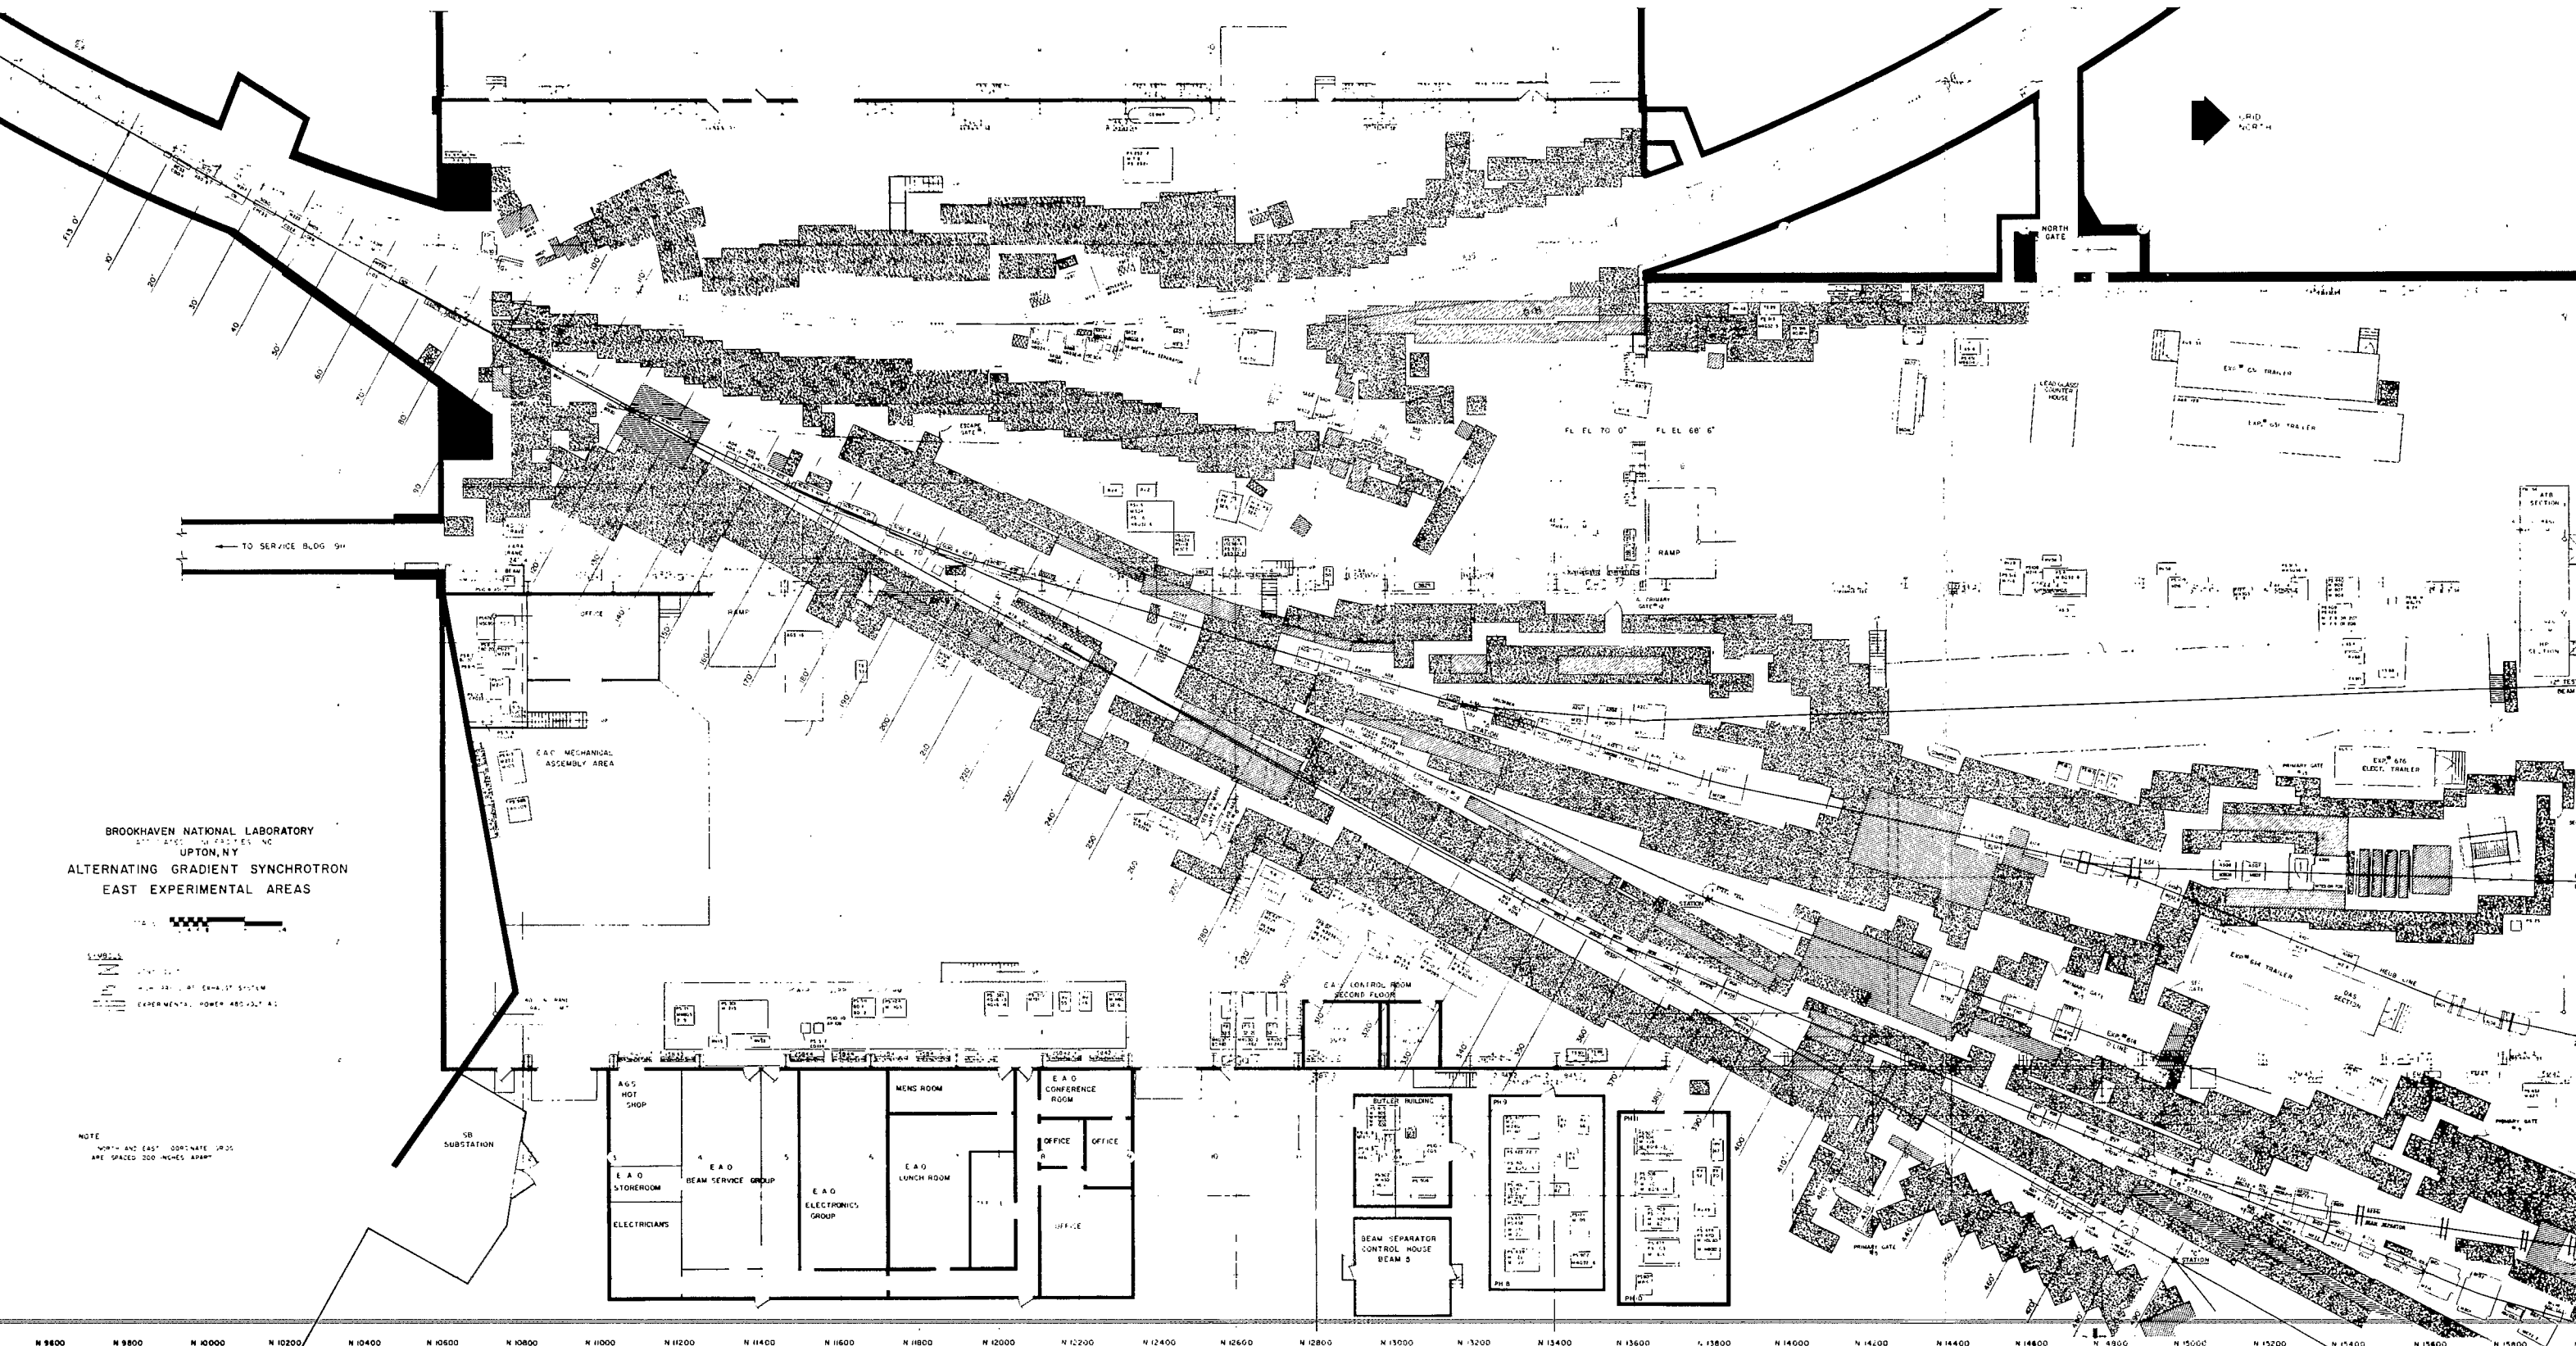


BROOKHAVEN NATIONAL LABORATORY  
 UPTON, N.Y.  
 ALTERNATING GRADIENT SYNCHROTRON  
 EAST EXPERIMENTAL AREAS



NOTE  
 NORTH AND EAST COORDINATE GRID  
 ARE SPACED 300 INCHES APART

N 9800 N 9900 N 10000 N 10200 N 10400 N 10600 N 10800 N 11000 N 11200 N 11400 N 11600 N 11800 N 12000 N 12200 N 12400 N 12600 N 12800 N 13000 N 13200 N 13400 N 13600 N 13800 N 14000 N 14200 N 14400 N 14600 N 14800 N 15000 N 15200 N 15400 N 15600 N 15800

FIG 1

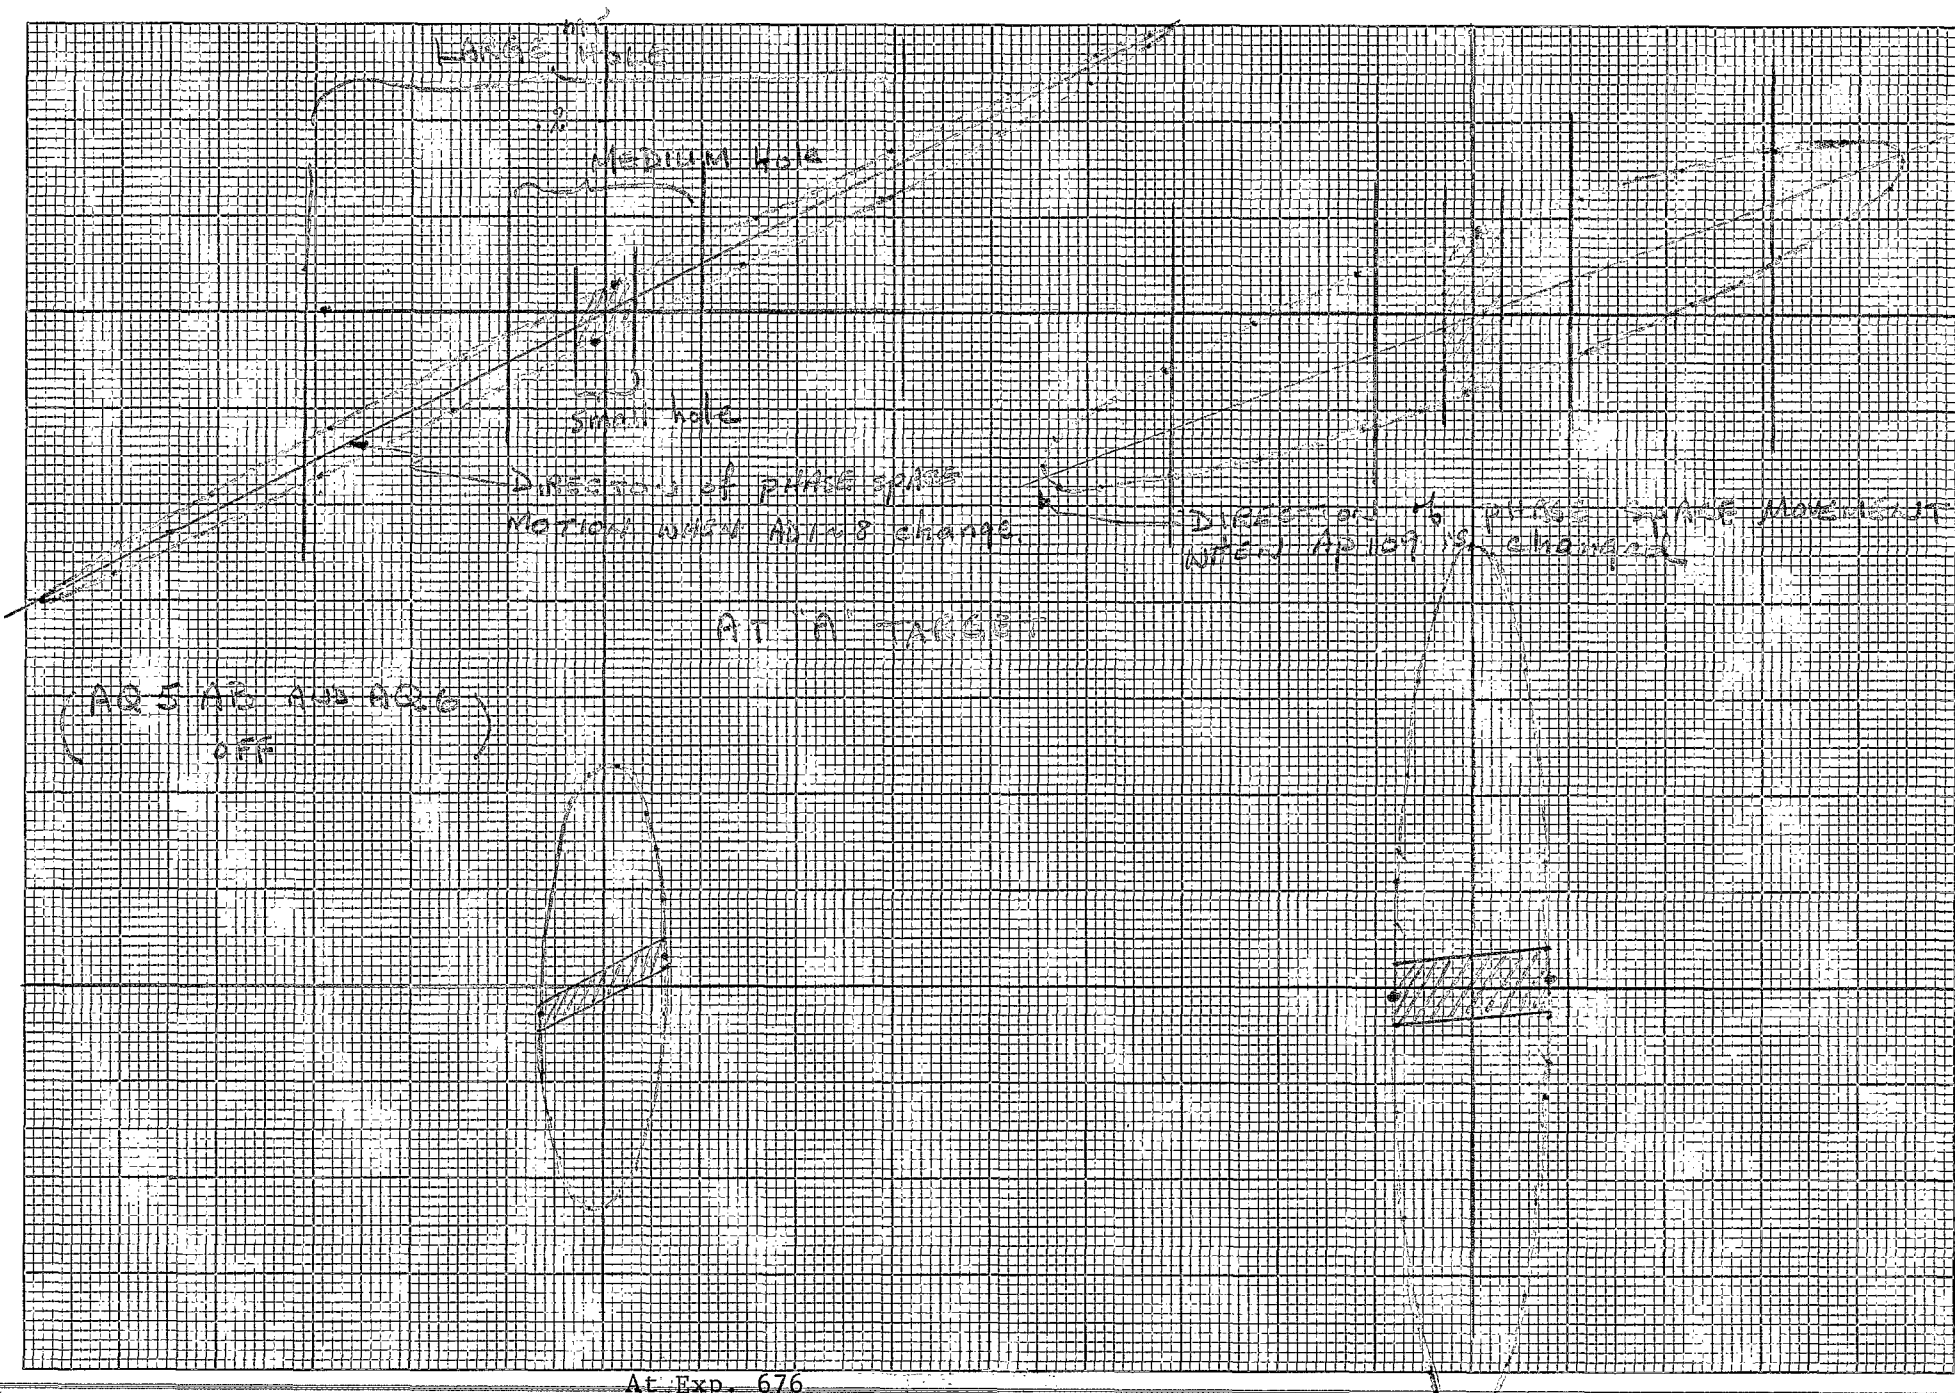

At Exp. 676

Fig. 2 Phase Ellipse at "A" Station and Exp. 676