

SENSITIVITY COMPARISON OF HELIUM LEAK DETECTOR VS MASS SPECTROMETER (RESIDUAL GAS ANALYZER)

J. C. Schuchman

November 1967

Collider Accelerator Department
Brookhaven National Laboratory

U.S. Department of Energy

USDOE Office of Science (SC)

Notice: This technical note has been authored by employees of Brookhaven Science Associates, LLC under Contract No.AT-30-2-GEN-16 with the U.S. Department of Energy. The publisher by accepting the technical note for publication acknowledges that the United States Government retains a non-exclusive, paid-up, irrevocable, world-wide license to publish or reproduce the published form of this technical note, or allow others to do so, for United States Government purposes.

DISCLAIMER

This report was prepared as an account of work sponsored by an agency of the United States Government. Neither the United States Government nor any agency thereof, nor any of their employees, nor any of their contractors, subcontractors, or their employees, makes any warranty, express or implied, or assumes any legal liability or responsibility for the accuracy, completeness, or any third party's use or the results of such use of any information, apparatus, product, or process disclosed, or represents that its use would not infringe privately owned rights. Reference herein to any specific commercial product, process, or service by trade name, trademark, manufacturer, or otherwise, does not necessarily constitute or imply its endorsement, recommendation, or favoring by the United States Government or any agency thereof or its contractors or subcontractors. The views and opinions of authors expressed herein do not necessarily state or reflect those of the United States Government or any agency thereof.

Accelerator Department
BROOKHAVEN NATIONAL LABORATORY
Associated Universities, Inc.
Upton, L.I., N.Y.

AGS DIVISION TECHNICAL NOTE

No. 41

J. C. Schuchman

Nov. 15, 1967

SENSITIVITY COMPARISON OF HELIUM LEAK DETECTOR VS MASS SPECTROMETER
(RESIDUAL GAS ANALYZER)

At the Conversion Parameter Working Committee Meeting of Sept. 20th, some questions were raised concerning the relative sensitivity of a mass spectrometer to that of a commercial helium leak detector, the thought being that perhaps either instrument could be used on the converted AGS vacuum system.


Tests were conducted comparing a commercially available 60° magnetic sector mass spectrometer (Veeco GA-4) to a helium leak detector of comparable design (Veeco MS-9).

The results show the leak detector to be 3 to 5 times more sensitive to helium than the mass spectrometer. The reason for this difference, even though both instruments are of similar design, is that the mass spectrometer baffles more of the ion current thereby reducing the sensitivity, but increasing the resolving power of the instrument. The leak detector uses less baffling and achieves higher sensitivity with reduced resolution.

Note: The GA-4 mass spectrometer can also make use of an electron multiplier for increased sensitivity. However, it is not as versatile when used this way and, therefore, was not considered in this test.

The response time of the leak detector for one-half superperiod (length of mockup) was also measured. It was less than three seconds with all twelve pumps operating.

Test Apparatus: "Mock-up" Conversion System in Bldg. 197

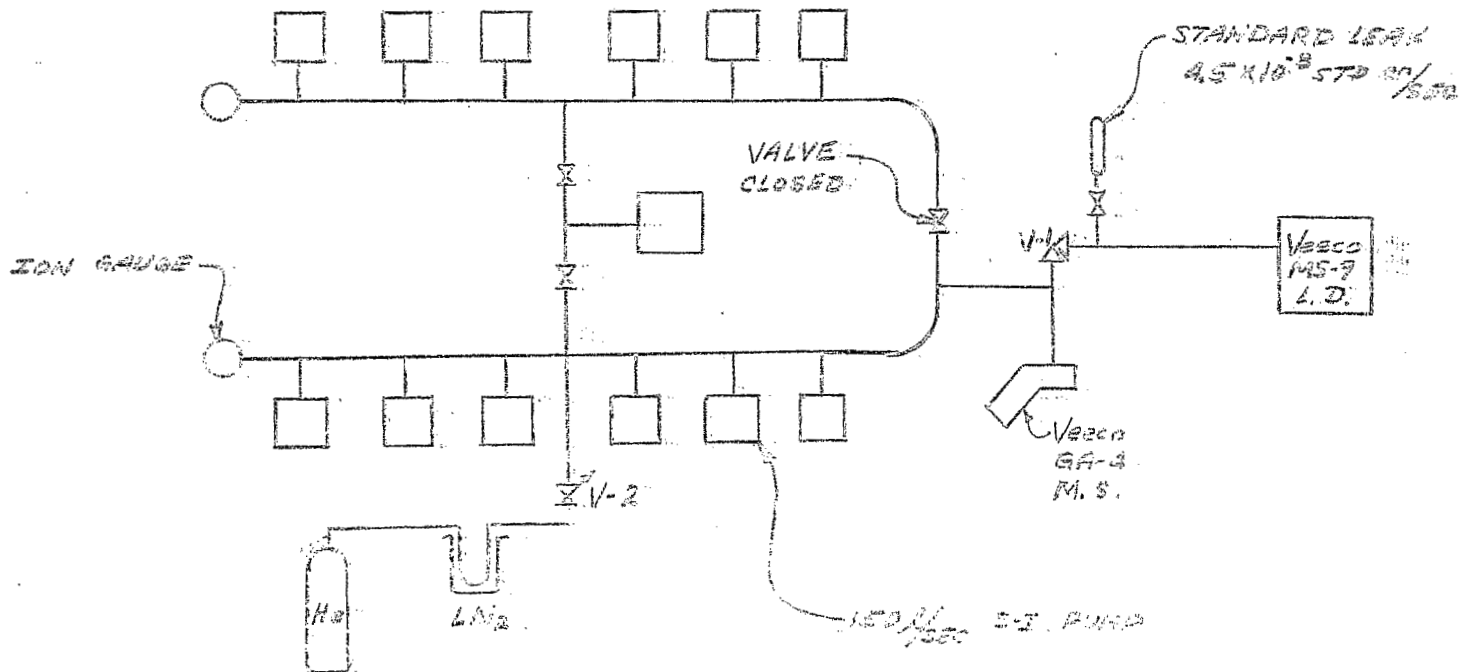

Test Procedure:

1. Calibrate leak detector with valve V-1 closed.
2. Open valve V-1 and adjust mass spectrometer zero to that of the leak detector.
3. Bleed-in helium through valve V-2 and record output signal change of L.D. and M.S.
4. Compare sensitivity of L.D. to M.S. by using $\text{Sen} = \frac{\text{change signal}}{\text{Change He partial press?}}$
assume the change in He partial press is the same
in both instruments compare the ratio:

$$\frac{\text{sensitivity L.D.}}{\text{sensitivity M.S.}}$$

Test Results


1. Leak detector sensitivity (minimum detectable leak) = 6.4×10^{-10} std. cc/sec.
2. It was not possible to maintain a steady pressure with the leak either opened or closed therefore points on either side of opening or closing the leak were used.

	(Δ signal) L.D. Scale divisions	(Δ signal) M.S. Scale divisions	Sensitivity Ratio $\frac{L.D.}{M.S.}$
Close valve	300-80 = 220	98-22 = 76	2.9
Open "	840-25 = 215	180-5 = 175	4.7
Close "	890-100 = 790	190-27 = 163	4.8
Open "	300-36 = 264	70 - 8 = 62	4.3
Open "	880-200 = 680	180-49 = 131	5.2
Close "	880-160 = 720	180-41 = 139	5.2

Note: All sputter-ion pumps remained operating during this test.

Response Time Measurement

The response time of the leak detector to a helium leak was also measured. Again the "mock-up" system was used, however, this time the entire system was used (1/2 superperiod). The leak detector was connected to one end of the system and a helium leak to the other as shown below:

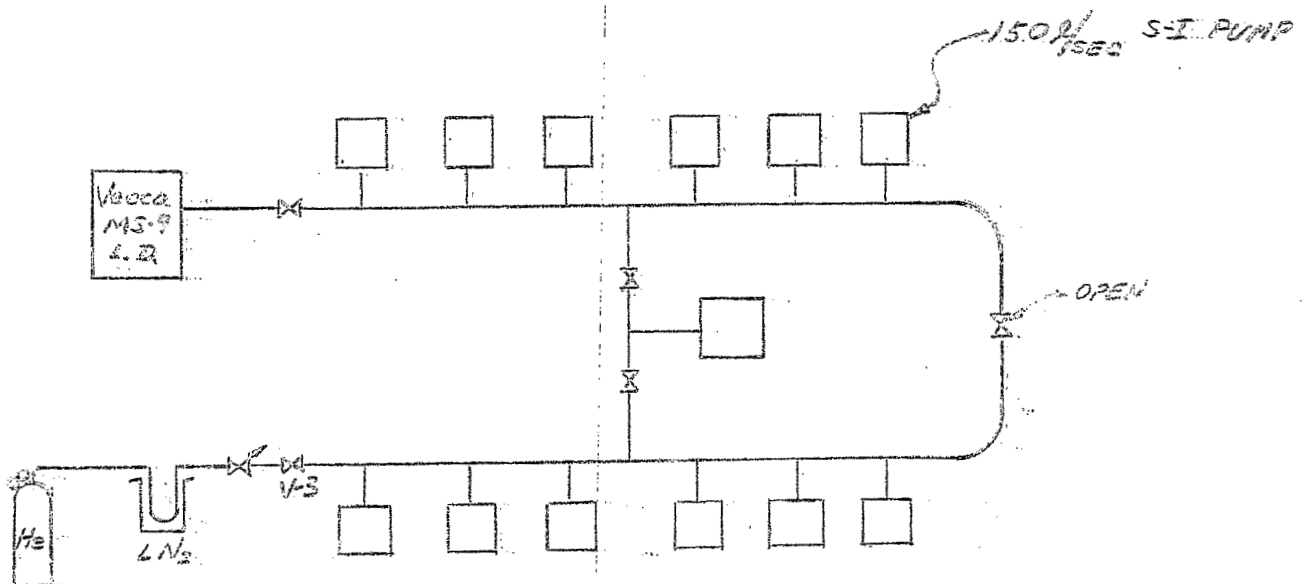

The system was pumped to a base pressure, valve V-3 was opened and the time recorded until a signal response was noted on the leak detector.

Test Results

Run #1 - Starting with a 50 scale division background due to residual helium in the system the response time was 2.9 sec. All twelve pumps were operating during this test. The helium leak size may be approximated by calculating the pumping speed at the leak due to the sputter-ion pump (using 150ℓ/sec for its speed) and measuring the change in pressure before and after opening the leak.

$$Q = s \Delta P = (61) (2.8 \times 10^{-5}) \text{ Tℓ/sec}$$

$$Q = 1.71 \times 10^{-3} \frac{\text{Tℓ}}{\text{sec}} = 2.3 \times 10^{-3} \text{ std cc/sec}$$

Run #2 Starting with a background of 70 scales the response time was 2.3 sec.

Run #3 Starting with a background of 62 scales the response time was 1.2 sec (larger leak used).

Distribution:

J.P. Blewett
G.K. Green
J.H. Lancaster
C. Lasky
M. Plotkin
I. Polk
J. Spiro
A. van Steenberg
G.W. Wheeler
R. Cool
R. Drucker
A. Marino
H. McChesney
J. Sanford
G. Stubbings
C. Gould
V. Buchanan
J.G. Cottingham
E.B. Forsyth
J.J. Grisoli
J.C. Schuchman