

DESIGN OF A VACUUM SYSTEM FOR SPARE DUOPLASMATRON ION SOURCES

P. Clarke

October 1968

Collider Accelerator Department
Brookhaven National Laboratory

U.S. Department of Energy

USDOE Office of Science (SC)

Notice: This technical note has been authored by employees of Brookhaven Science Associates, LLC under Contract No.AT-30-2-GEN-16 with the U.S. Department of Energy. The publisher by accepting the technical note for publication acknowledges that the United States Government retains a non-exclusive, paid-up, irrevocable, world-wide license to publish or reproduce the published form of this technical note, or allow others to do so, for United States Government purposes.

DISCLAIMER

This report was prepared as an account of work sponsored by an agency of the United States Government. Neither the United States Government nor any agency thereof, nor any of their employees, nor any of their contractors, subcontractors, or their employees, makes any warranty, express or implied, or assumes any legal liability or responsibility for the accuracy, completeness, or any third party's use or the results of such use of any information, apparatus, product, or process disclosed, or represents that its use would not infringe privately owned rights. Reference herein to any specific commercial product, process, or service by trade name, trademark, manufacturer, or otherwise, does not necessarily constitute or imply its endorsement, recommendation, or favoring by the United States Government or any agency thereof or its contractors or subcontractors. The views and opinions of authors expressed herein do not necessarily state or reflect those of the United States Government or any agency thereof.

Accelerator Department
BROOKHAVEN NATIONAL LABORATORY
Associated Universities, Inc.
Upton, L.I., N.Y.

AGS DIVISION TECHNICAL NOTE

No. 55

P. Clarke
October 8, 1968

DESIGN OF A VACUUM SYSTEM FOR SPARE DUOPLASMATRON ION SOURCES

1) Objective

To design a vacuum system to test and hold AGS spare duoplasmatron ion sources. The system should be failsafe and maintenance free.

2) Principle

The main criterion for the vacuum system is that an oxide cathode can be outgassed, activated and held for long periods as an AGS machine spare.

The major outgassing products from an oxide cathode during activation are water vapor and carbon monoxide. These gases must be pumped to a pressure less than 10^{-5} torr. There must be no hydrocarbon contamination from the vacuum system or pumps. Many vacuum systems can do this job but sorption pumps are ideal.

Sorption pumps when cooled to liquid nitrogen temperature can reduce the total pressure in a vacuum system to less than 10^{-2} torr. The particle pressure of gases like H_2O , CO , N_2 , Ar and O_2 are reduced to pressures less than 10^{-5} torr while gases like H_2 , Ne and He are only reduced to pressures less than 10^{-2} torr. It is these latter gases with low activation energies for sorption that make the total pressure in sorption pumped vacuum systems when the starting gas is air at atmospheric pressure.

3) Vacuum System Design and Tests

The vacuum system is shown in Fig. 1. Each sorption pump holds about two pounds of zerolite. One pump was charged with Linde molecular sieve #13X, the other with Linde molecular sieve #5A. The molecular sieve #13X seemed to pump the outgassing products from the filament at liquid nitrogen temperature better than molecular sieve #5A. This observation needs further testing.

The filament was outgassed slowly by carefully increasing the filament heater current until the ion source T.C. gauge indicated 200 microns. As the filament outgassed, the pressure was held at 200 microns by adjusting the filament heater current. The T.C. gauge above the sorption pump never rose above 20 microns.

The filament was considered outgassed when the filament heater current read 28 amp and the ion source T.C. gauge indicated 25 microns.

After the filament was outgassed, the valve above the sorption pump was closed and H_2 leaked into the vacuum system through a heated Pd leak. When the pressure in the vacuum system indicated 200 microns, the Pd leak was cooled and the pressure stabilized at 200 microns. The ion source was then pulsed at 250 volts and a 25 amp arc discharge was established in the ion source.

The ion source was isolated from the sorption pump by the closed valve and so could be considered a vacuum tube with no sources or sinks of gas (almost). The only attention the system needs is to leak in H_2 gas periodically because the H_2 is ion pumped in the source.

Life test data is not available. The first filament operated normally for 36 hours before installation in the AGS linac.

Distr: Department Administration
AGS Division Staff

BY *P. C. ...* DATE *...*
CHKD. BY _____ DATE _____

SUBJECT *Vacuum System for Pd-100
Spring Equilibrium Torq. Source*
DEPT. OR PROJECT _____

SHEET NO. _____ OF _____
JOB NO. _____

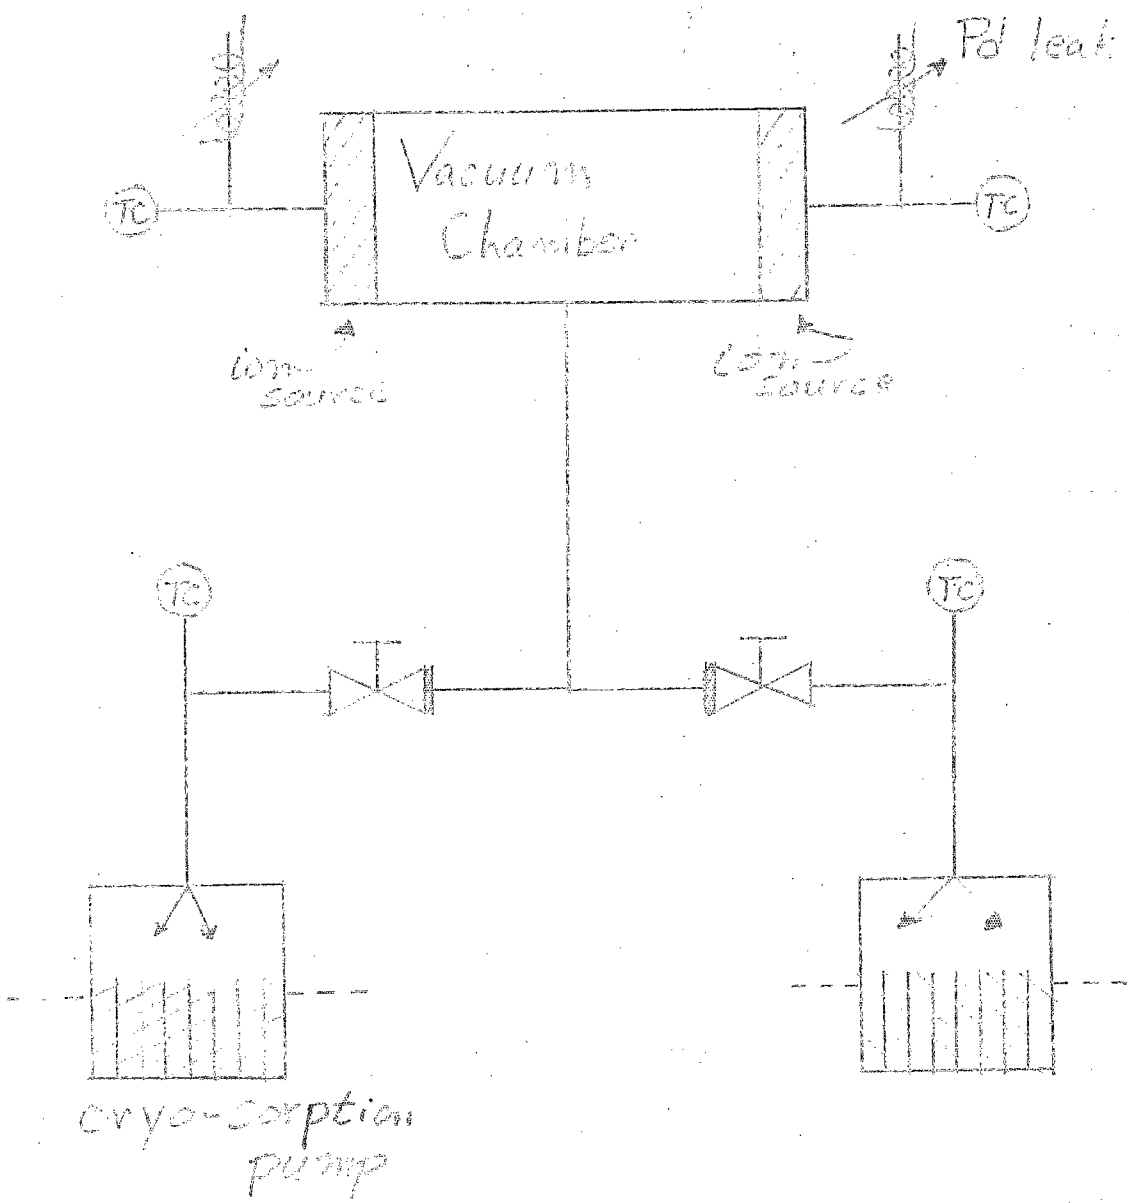


Figure 1