



BNL-105798-2014-TECH

EP&S No. 83;BNL-105798-2014-IR

Calibration of magneto-resistive probes in A1D5 and A1D6 (Beam spectrometer magnets)

H. N. Brown

April 1978

Collider Accelerator Department
Brookhaven National Laboratory

U.S. Department of Energy

USDOE Office of Science (SC)

Notice: This technical note has been authored by employees of Brookhaven Science Associates, LLC under Contract No.EY-76-C-02-0016 with the U.S. Department of Energy. The publisher by accepting the technical note for publication acknowledges that the United States Government retains a non-exclusive, paid-up, irrevocable, world-wide license to publish or reproduce the published form of this technical note, or allow others to do so, for United States Government purposes.

DISCLAIMER

This report was prepared as an account of work sponsored by an agency of the United States Government. Neither the United States Government nor any agency thereof, nor any of their employees, nor any of their contractors, subcontractors, or their employees, makes any warranty, express or implied, or assumes any legal liability or responsibility for the accuracy, completeness, or any third party's use or the results of such use of any information, apparatus, product, or process disclosed, or represents that its use would not infringe privately owned rights. Reference herein to any specific commercial product, process, or service by trade name, trademark, manufacturer, or otherwise, does not necessarily constitute or imply its endorsement, recommendation, or favoring by the United States Government or any agency thereof or its contractors or subcontractors. The views and opinions of authors expressed herein do not necessarily state or reflect those of the United States Government or any agency thereof.

BROOKHAVEN NATIONAL LABORATORY
Associated Universities, Inc.
Upton, New York

EP&S DIVISION TECHNICAL NOTE
NO. 83

H. Brown
April 26, 1978

BNL USE ONLY

CALIBRATION OF MAGNETO-RESISTIVE PROBES IN AID5
AND AID6 (BEAM SPECTROMETER MAGNETS)

The vertical magnetic field in each magnet was measured with Hall Probe #731, operated at $I_H = 0.200000 \pm 0.000005$ Amps, placed on the bore axis about 27" inside the effective edge of the magnetic field (this is $\sim 18''$ from the center of the magnet). This Hall Probe was calibrated against an NMR fluxmeter in early 1977 by J. Weisenbloom. It was recalibrated by him against the NMR on 3 Dec. '77. This data went to about 20 kG. The calibration was "extended" to ~ 25 kG by using 3 Hall voltages measured in AID6 on 19 Sept. '77 and by deducing the corresponding fields B from the Danby, Jackson, Weisenbloom (DJW) measurements of B/I on that magnet. Due to uncertainties in current relationships between the DJW measurements and the present ones, the uncertainties in the extended calibration points increase to $\sim 0.25\%$ from 20 to 25 kG.

All of these calibration points (48 in all) were fitted to a 7th degree polynomial which was then used to convert all measured Hall Probe voltages to magnetic field. The fitting procedure minimized the squares of the relative deviation of the polynomial value from the measured field, i.e.

$$\sum_i \left(\frac{B(E_i) - B_i}{B_i} \right)^2$$

where B_i is the field measured at the corresponding Hall voltage E_i , and $B(E_i)$ is the value of the polynomial for the argument E_i . The resultant RMS deviation is $\pm 0.56 (10^{-3})$ for the 7th degree fit. This deviation is due primarily to a systematic difference between the first and second calibration runs, with the latter giving lower field values at the same

Hall voltage, by about 0.1%. This is plainly shown by the plot of $\left(\frac{B_i}{B(E_i)}\right)$ vs E in Fig. 1.

Measurements of B and the magneto-resistive probes (MR) in AID5 and AID6 were made at several different times between June and December 1977. The Hall voltages observed, after small corrections for probe current drifts, were all converted to kG via the polynomial described above. The MR probe voltages (4 in AID5 and 3 in AID6) were recorded, and the probe currents were monitored as well. The initial adjustment of the MR probe currents was made by setting them such that the probe voltage was close to 30 mV at zero magnetic field (really, zero current) in the magnet, i.e., $MR(B=0) \approx 30.000$ mV. The corresponding probe current I_o was also recorded. Both these observed values were used for later corrections.

The field measurement made by these probes is, of course, derived from the dependence of the resistance of the copper wire on B. However, the calibration curves and fits given here are in terms of the potential which would exist across the probe at the field B if the current in the probe were such that the potential would be exactly 30.000 mV at zero field. Therefore, since the initial setting $MR(B = 0)$ was not always exactly 30, and since the probe current drifted slightly anyway, all

observed MR readings were corrected as follows.

$$MR_{\text{corr.}}(B) = 30 \cdot \frac{R(B)}{R(B=0)} = 30 \cdot \left(\frac{MR_{\text{obs}}(B)}{I_{\text{obs}}} \right) \left(\frac{I_o}{MR(B=0)} \right)$$

It is this MR_{corr} which applies to the accompanying graphs and polynomial fits. In the graphs, in order to display the data with greater resolution, the field B has been divided by the empirical normalizing factor $(MR_{\text{corr}} - 30)^{.6954}$ and plotted as the ordinate versus $(MR_{\text{corr}} - 30)$ on the abscissa. Representative estimated errors in the measured points are shown. At low fields, they

are due mostly to the reading accuracy of MR(B) and of MR(B = 0). This was taken to be an RMS value of 2.8 μ V for the DVM employed. At intermediate fields, the error is mostly due to the $\pm 0.056\%$ deviation from the fit to the Hall probe calibration data. Above 20 kG, the estimated error grows to $\pm 0.25\%$ due to uncertainty in the "extended" calibration points derived from the DJW data.

The solid curves in the graphs are from 6th or 7th degree polynomial fits of B as a function of ($MR_{\text{corr}} - 30.$). The coefficients for these polynomials are listed in the tables.

To make use of these graphs or polynomials to their ultimate accuracy, the observed MR(B) voltage must first be corrected, as described above, before being converted to magnetic field B.

Finally, having determined the central field on axis from these calibrations, one can get the integrated field by multiplying by $L_{\text{eff}} \equiv \left(\int B d\ell \right) / B$. The effective lengths of D5 and D6 are plotted in the last graph as a function of B. This data is taken directly from simultaneous measurements of $\int B d\ell$ and B by DJW in the two magnets. Fits to those points are also plotted, and the polynomial coefficients listed in the tables.

Distr.: MPS Users

CALIBRATION OF HALL PROBE #731 AT $I = 0.200000 \pm .000005$ AMP.

RATIO OF MEASURED FIELDS TO POLYNOMIAL FIT

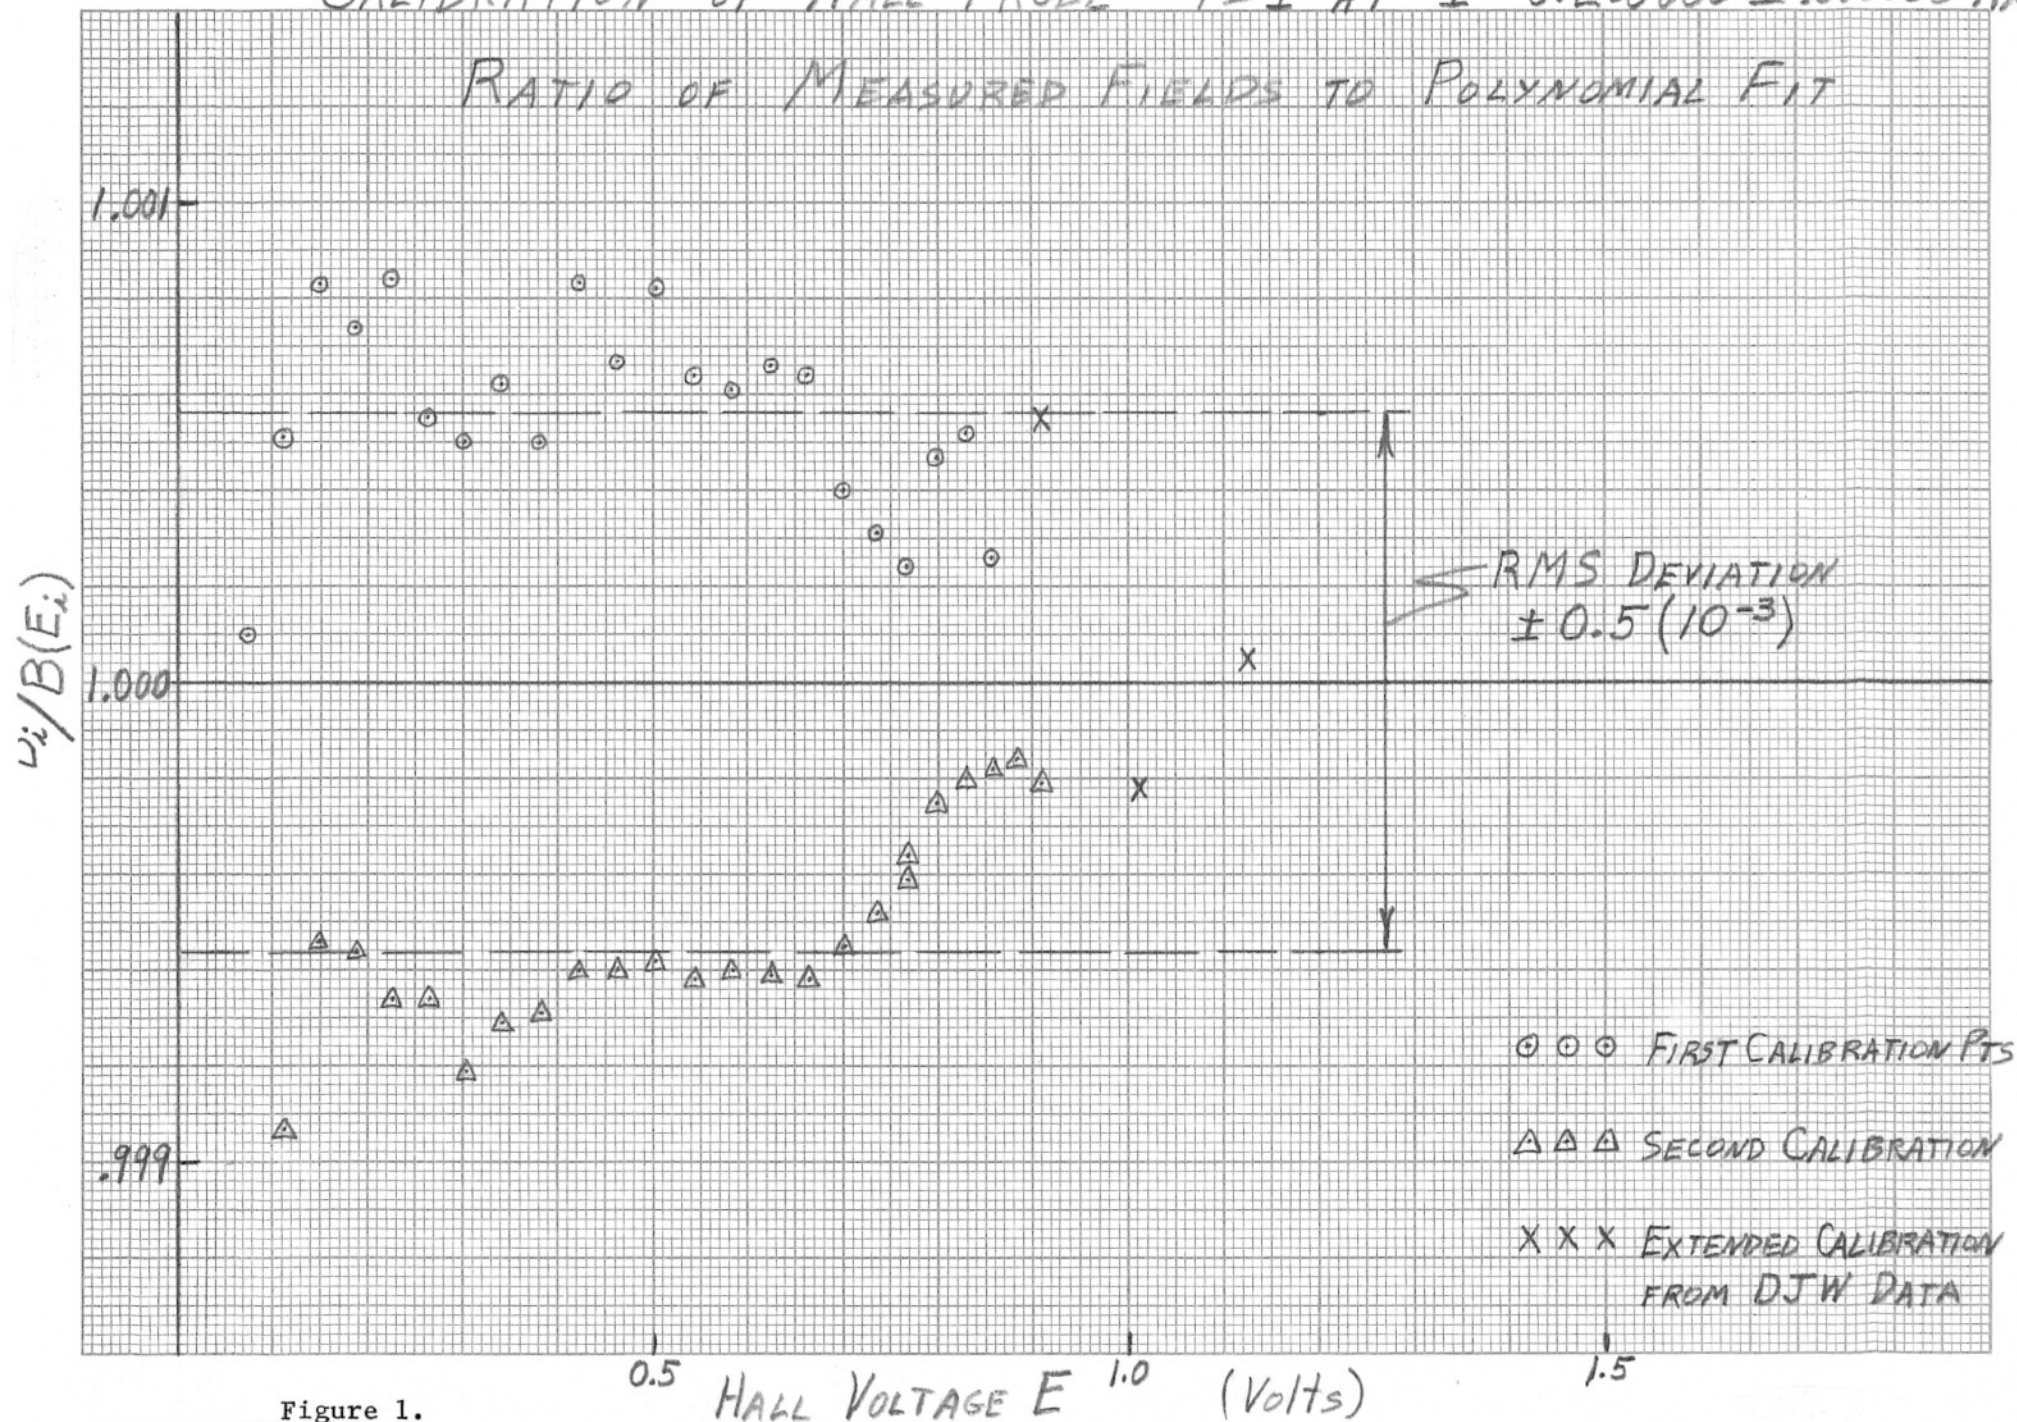


Figure 1.

20 APR 78

AID5 B vs MR1 CORRECTED

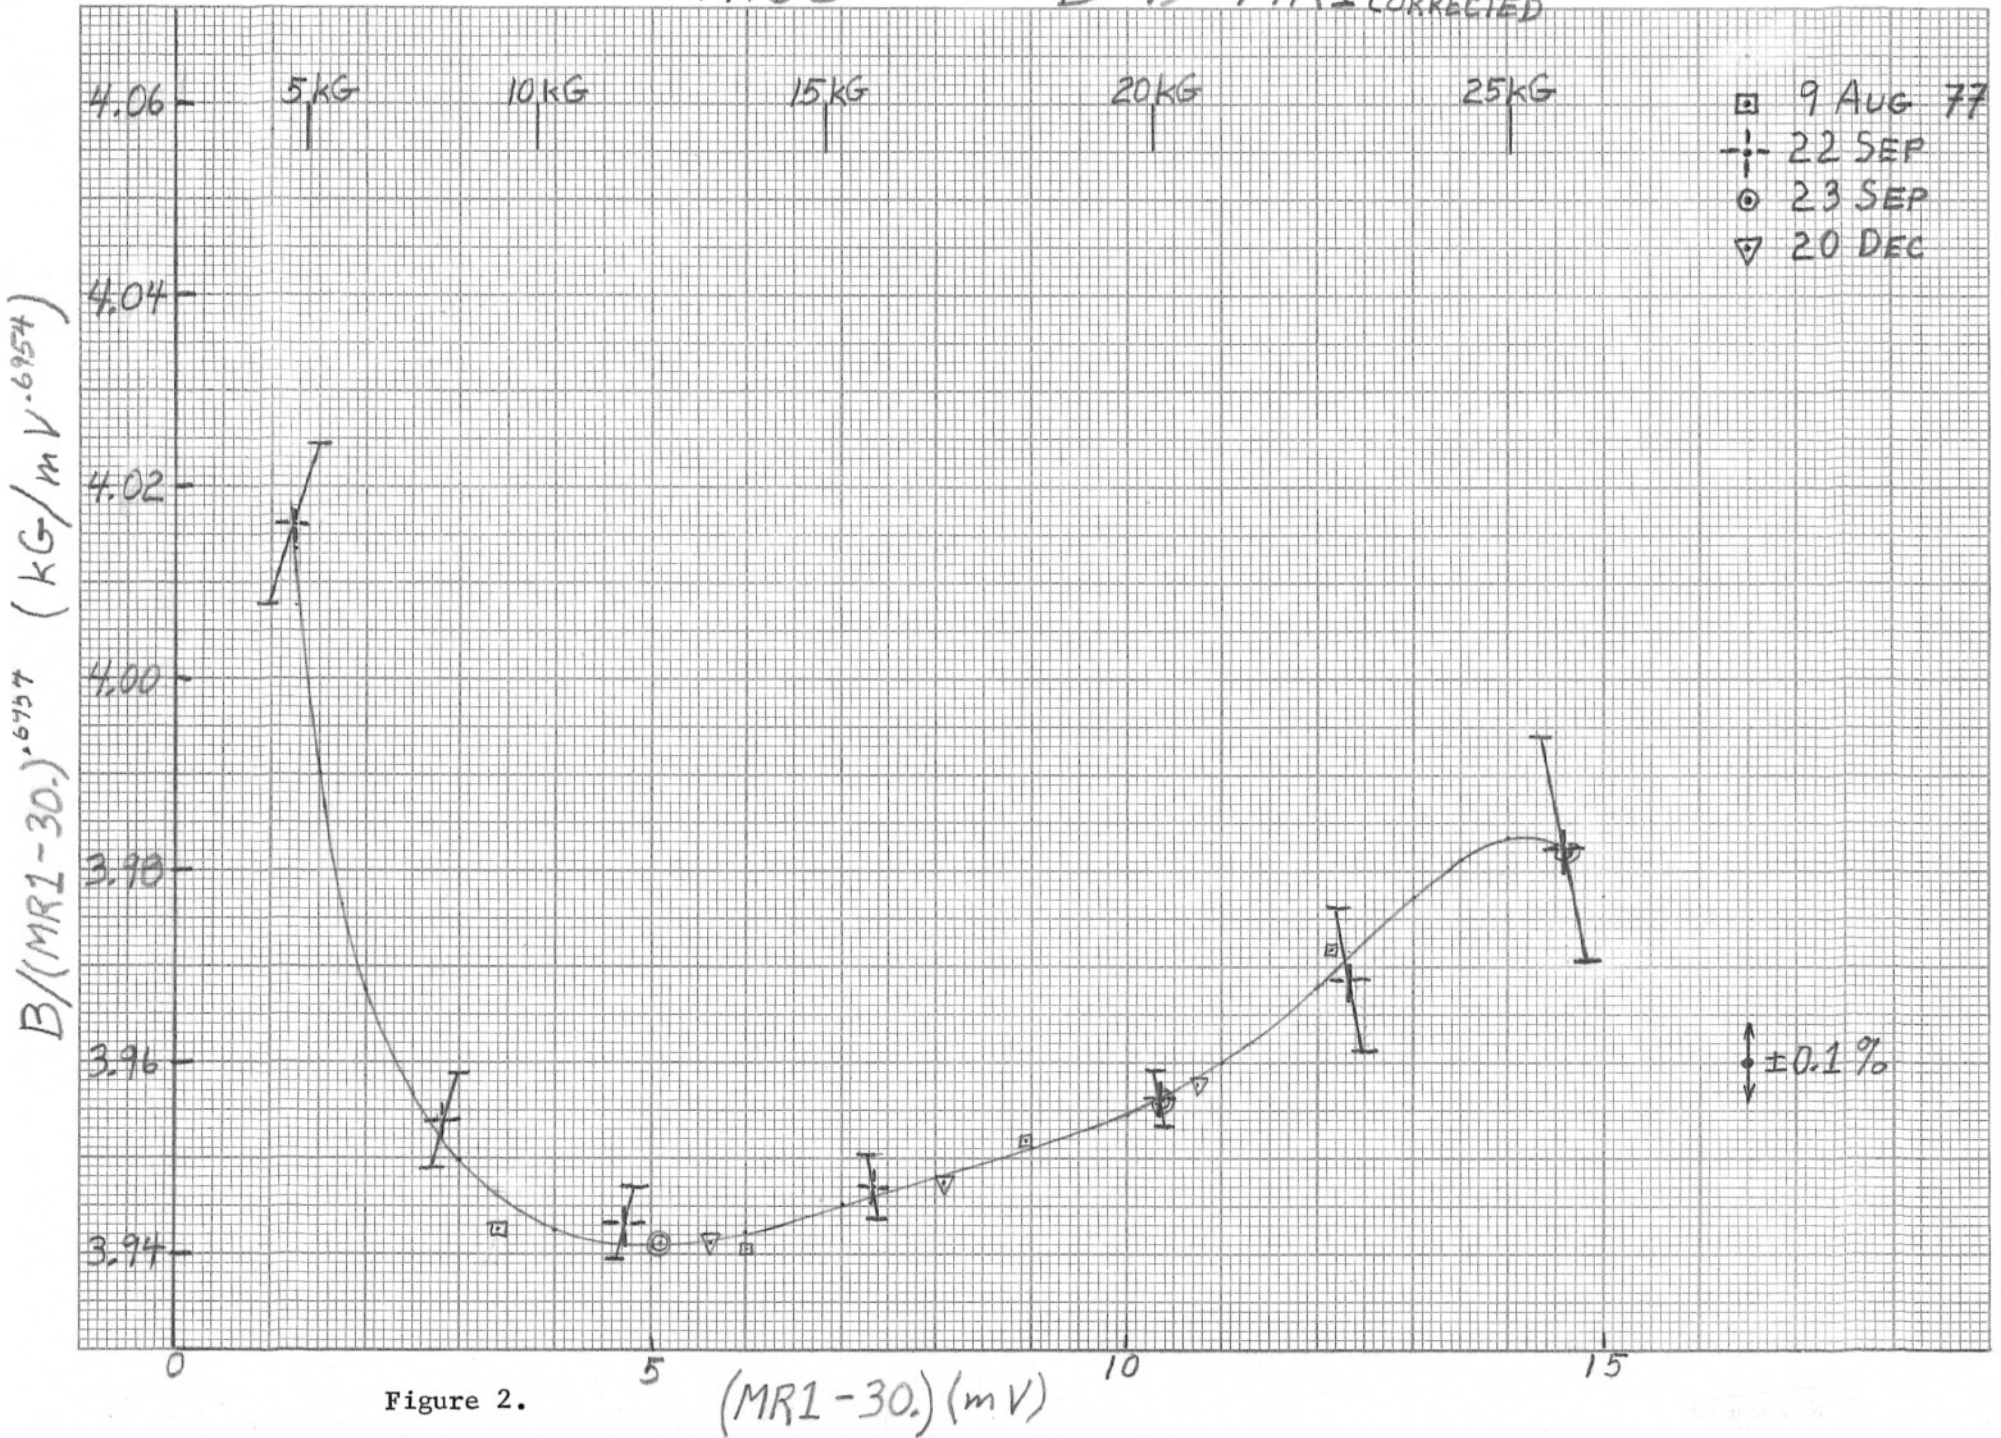


Figure 2.

20 APR 78

AID5 B vs MR2 CORRECTED

$B / ((MR2 - 30.) \cdot 0.6954)$ (KG/mV^{0.6954})


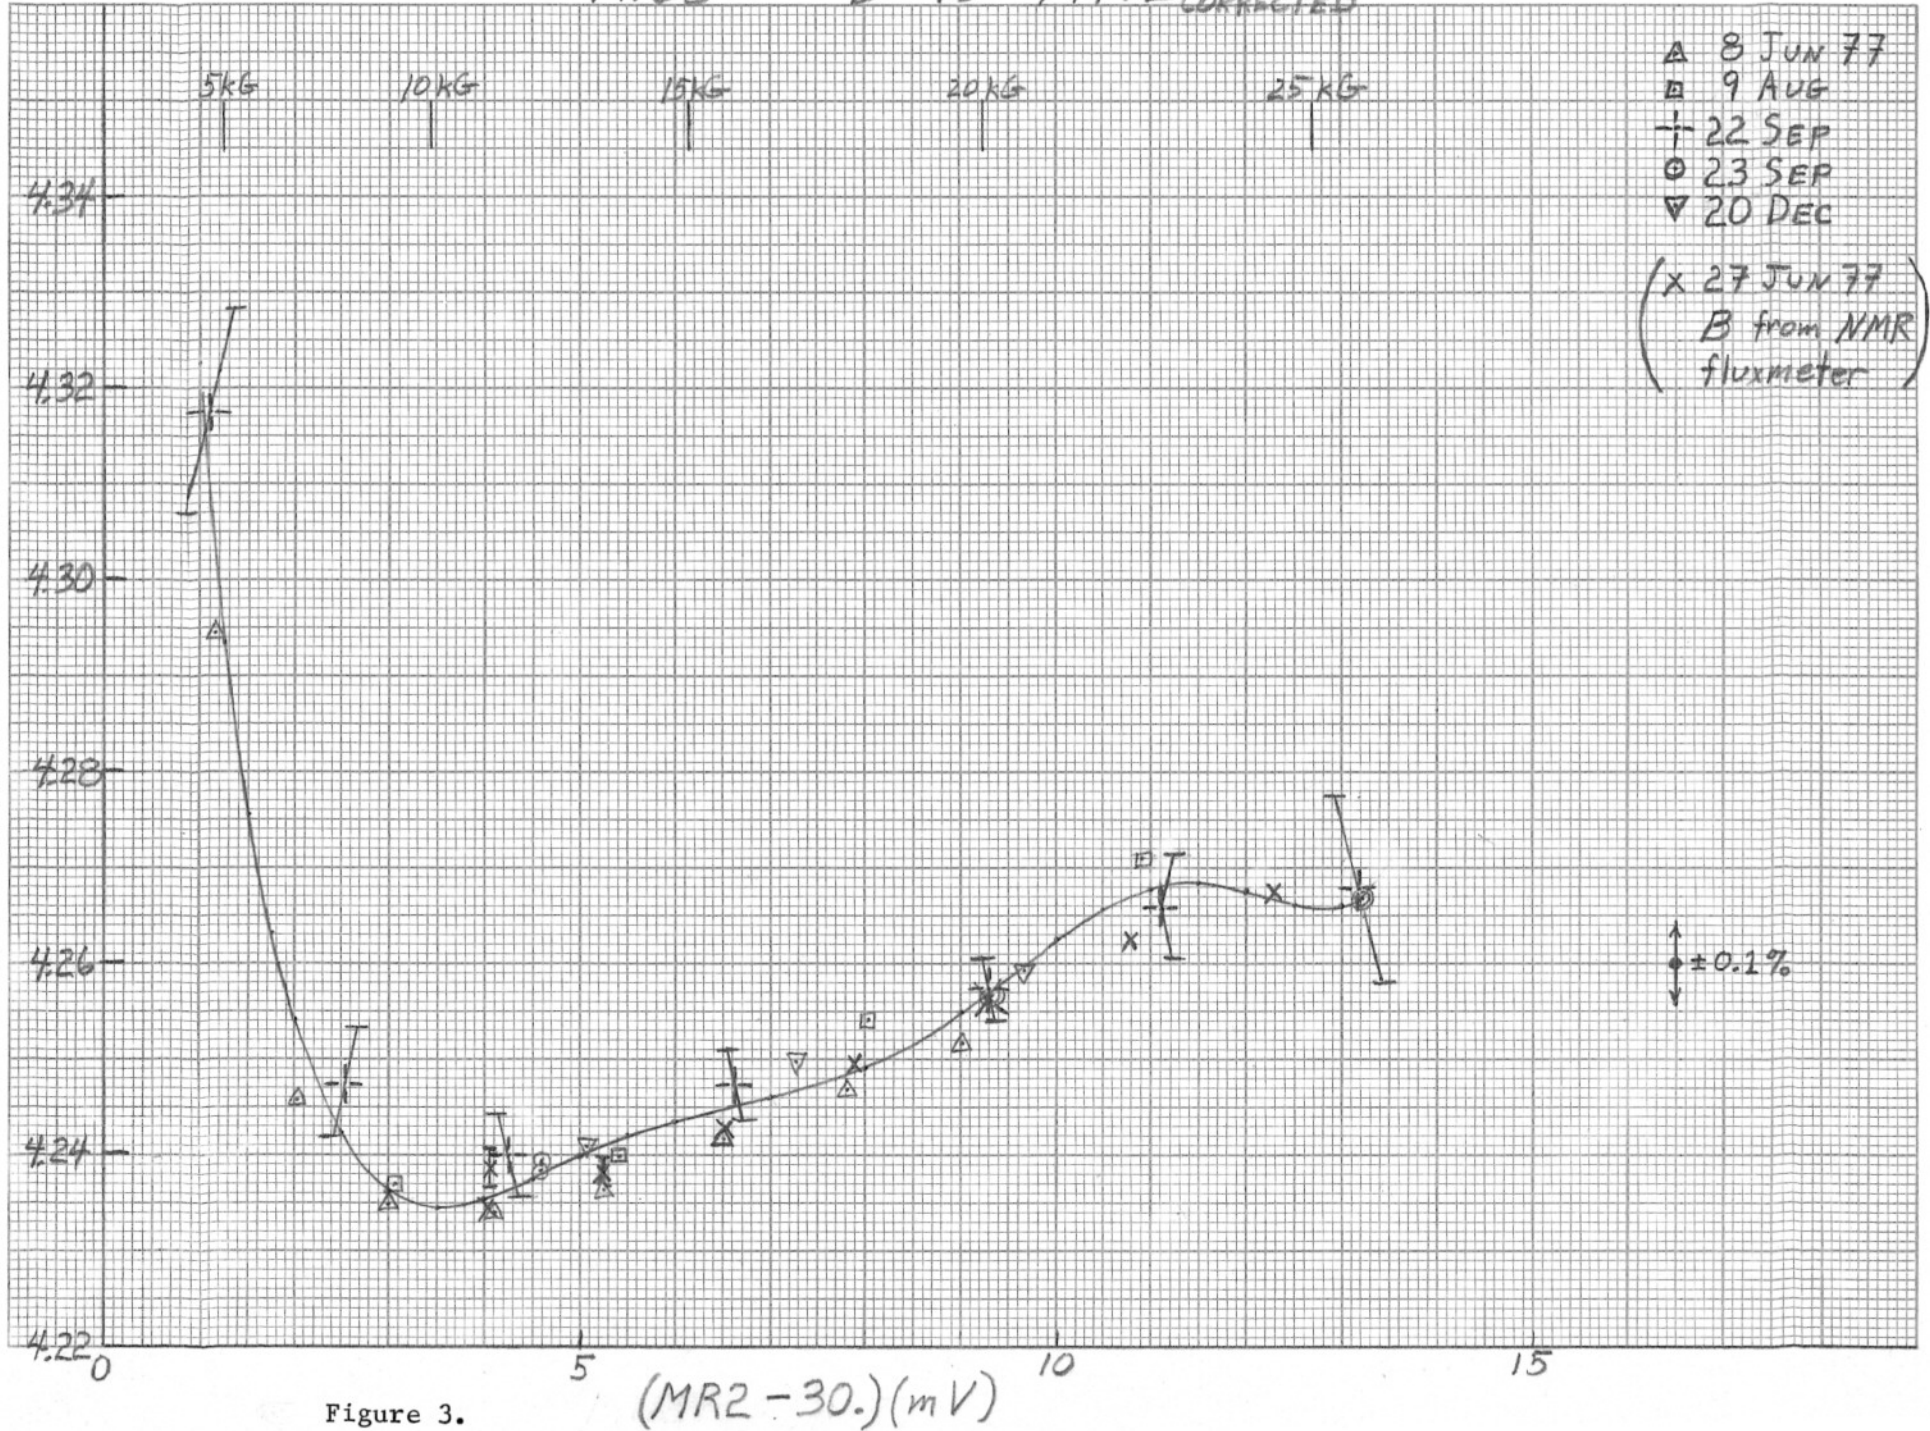


Figure 3.

20 APR 78

A1D5 B vs MR3 CORRECTED

B / (MR3 - 30.) °C/T (KG / mV · 0.6954)

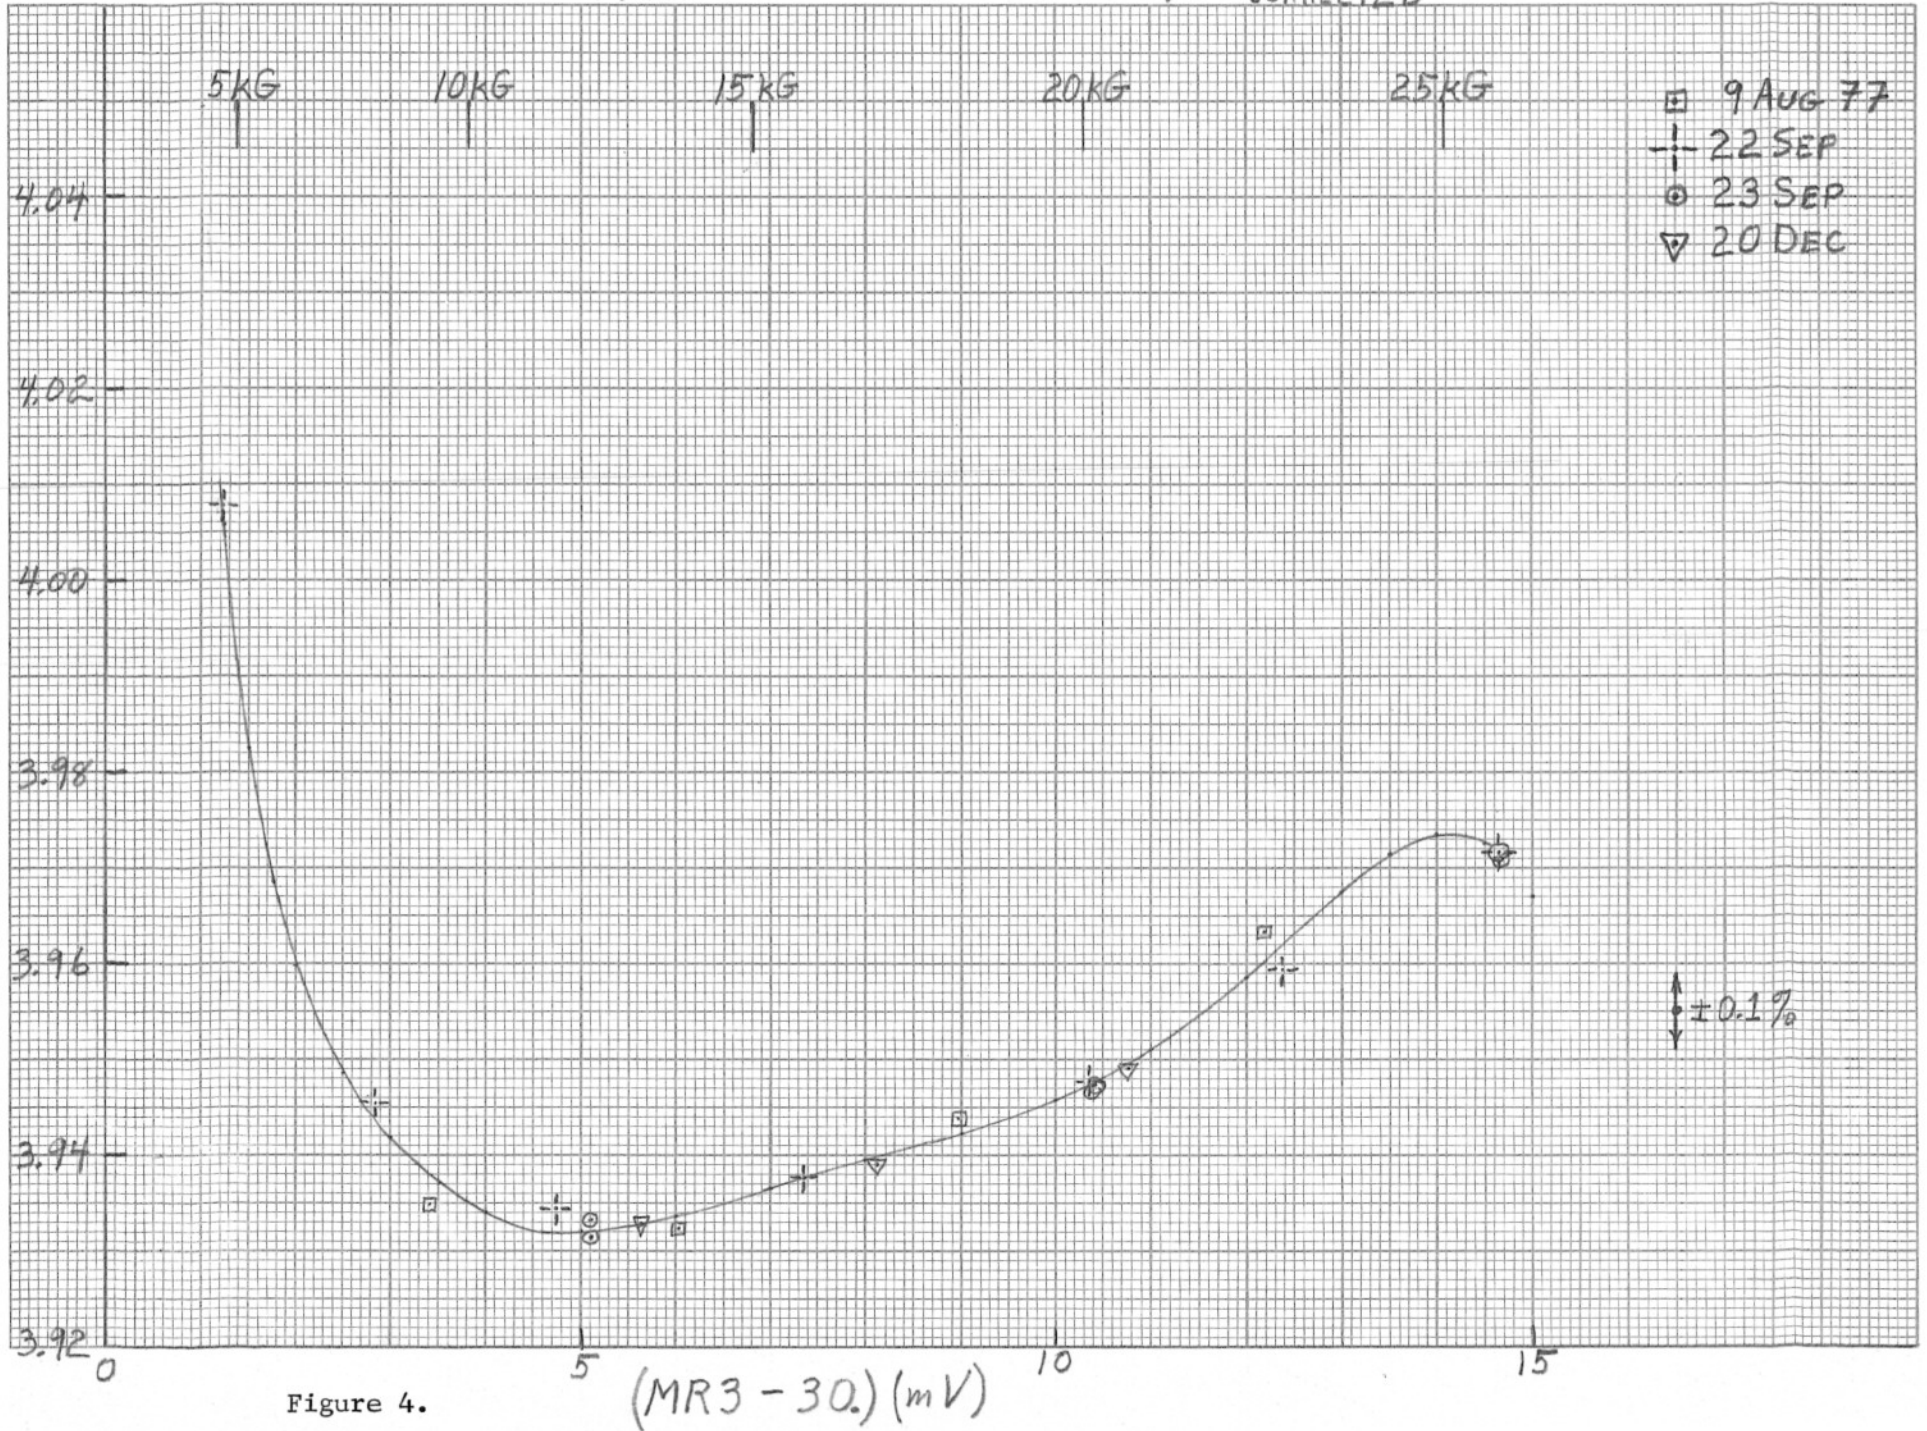

A1D5 B vs MR4 CORRECTED

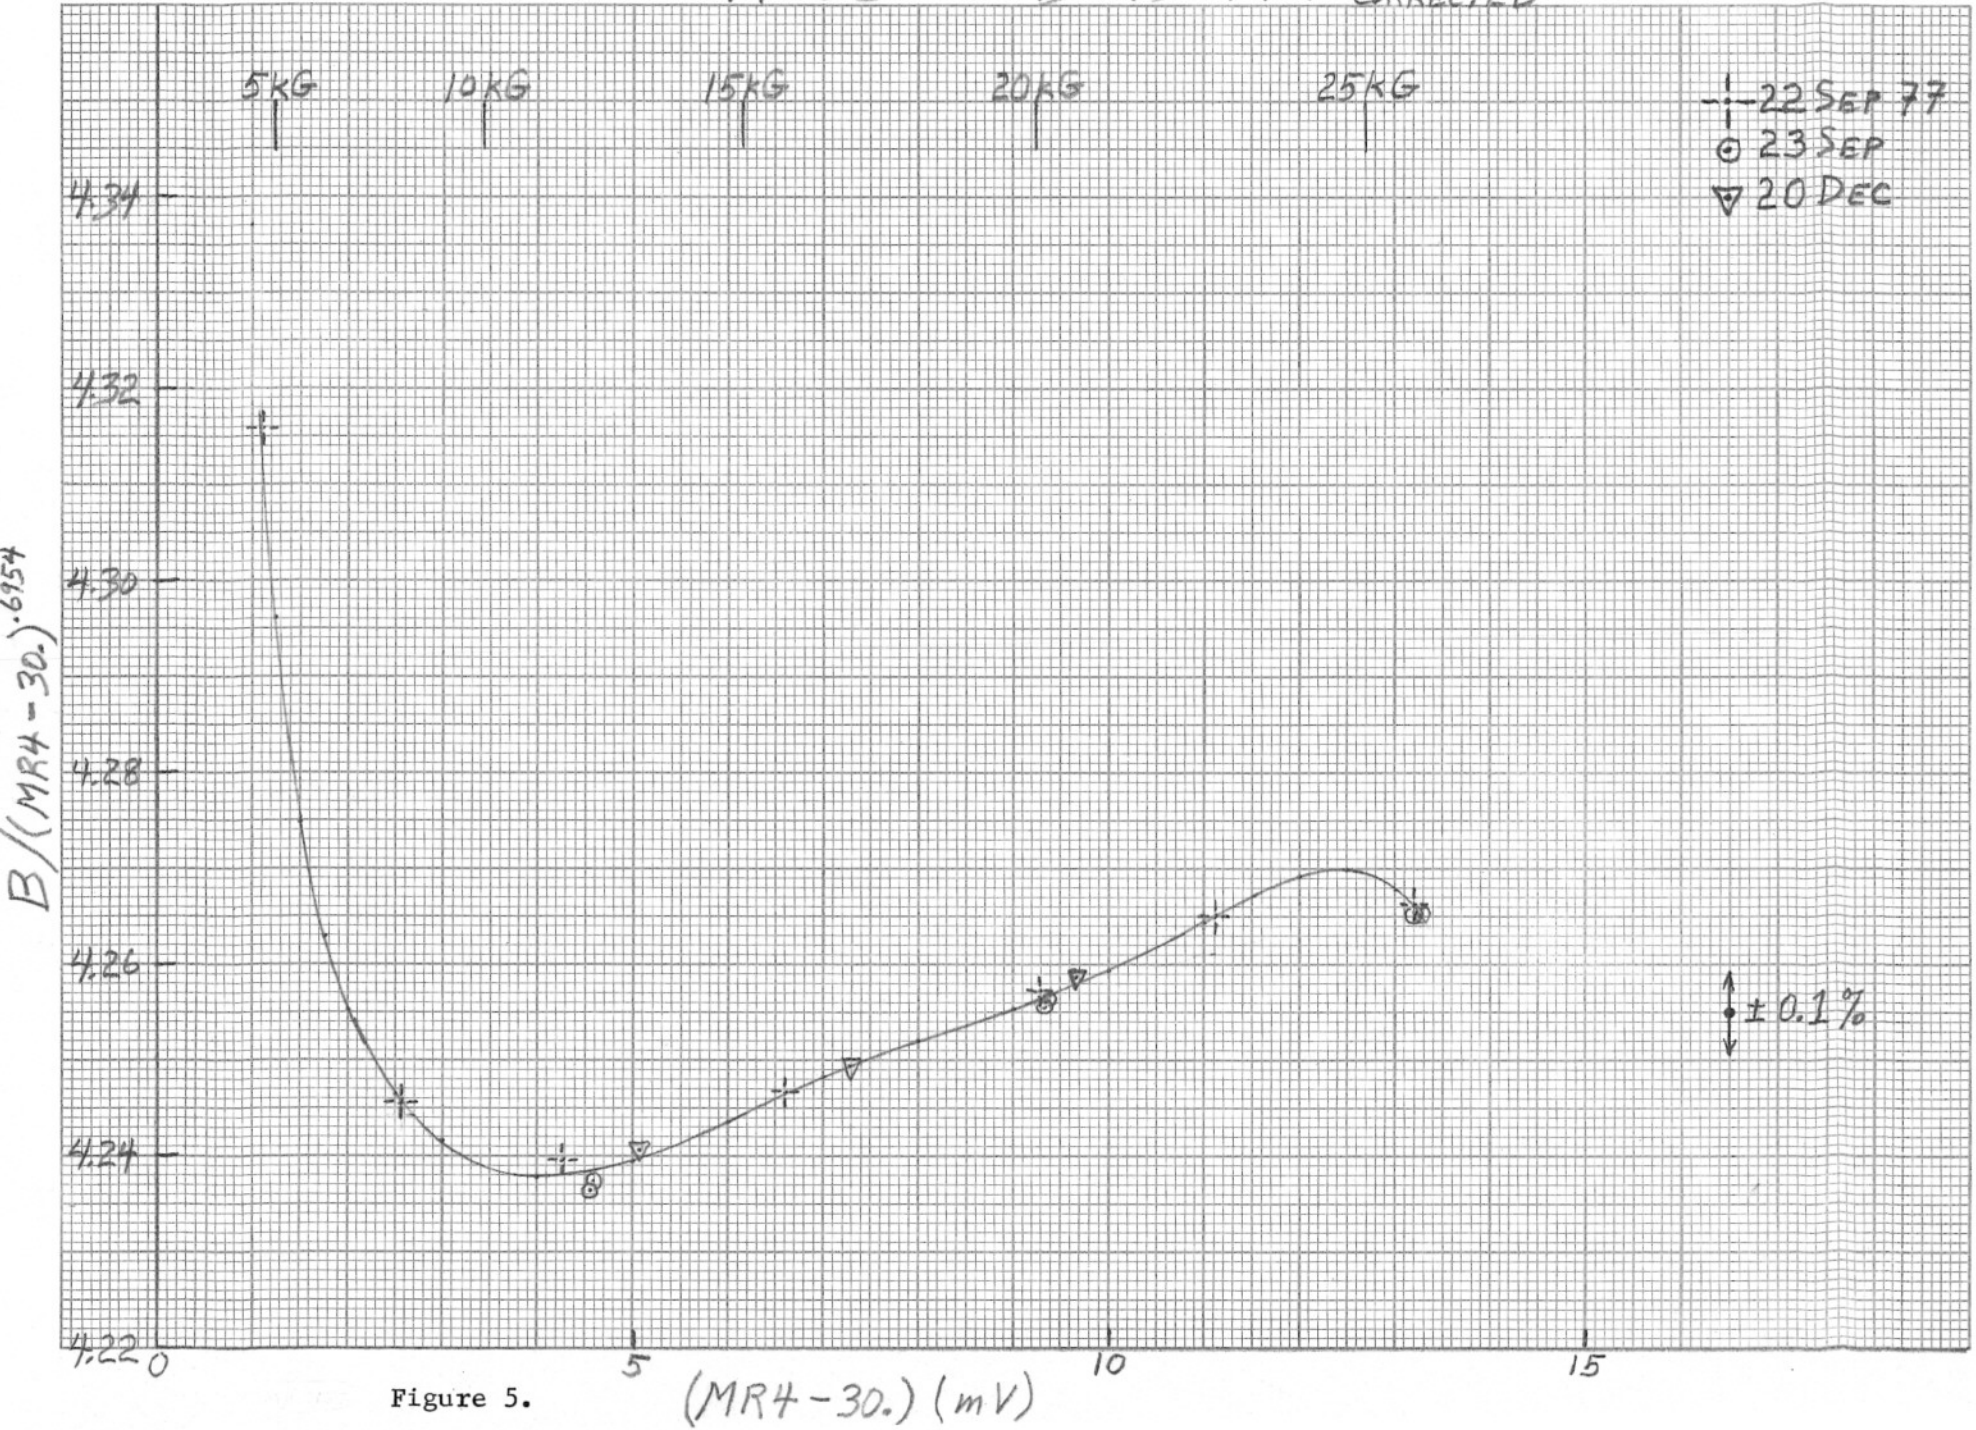


Figure 5.

Table I

A1D5

$$B = \sum_{k=0}^7 a_k (MR_{corr} - 30.)^k$$

<u>Coeff.</u>	<u>MR1</u>	<u>MR2</u>	<u>MR3</u>	<u>MR4</u>
a ₀	1.19031090	1.00293220	1.18639170	1.22780620
a ₁	3.20094900	3.91640470	3.19794770	3.48769200
a ₂	-.38512745	-.74724211	-.38626856	-.44009803
a ₃	.55883734E-1	.17463480	.56153340E-1	.67896426E-1
a ₄	-.51064311E-2	-.26486434E-1	-.51309232E-2	-.66301727E-2
a ₅	.25151483E-3	.23654323E-2	.25241344E-3	.35018683E-3
a ₆	-.50472288E-5	-.11250805E-3	-.50572813E-5	-.75861938E-5
a ₇	0.	.21888998E-5	0.	0.

$$L_{eff} = \sum_{k=0}^2 c_k B^k$$

c ₀	90.150420
c ₁	-.82048386E-2
c ₂	.20079110E-3

20 Apr 78

A1D6 B vs MR1 CORRECTED

$B/(MR1-30.)^{0.001}$ (KG/MV^{0.001})

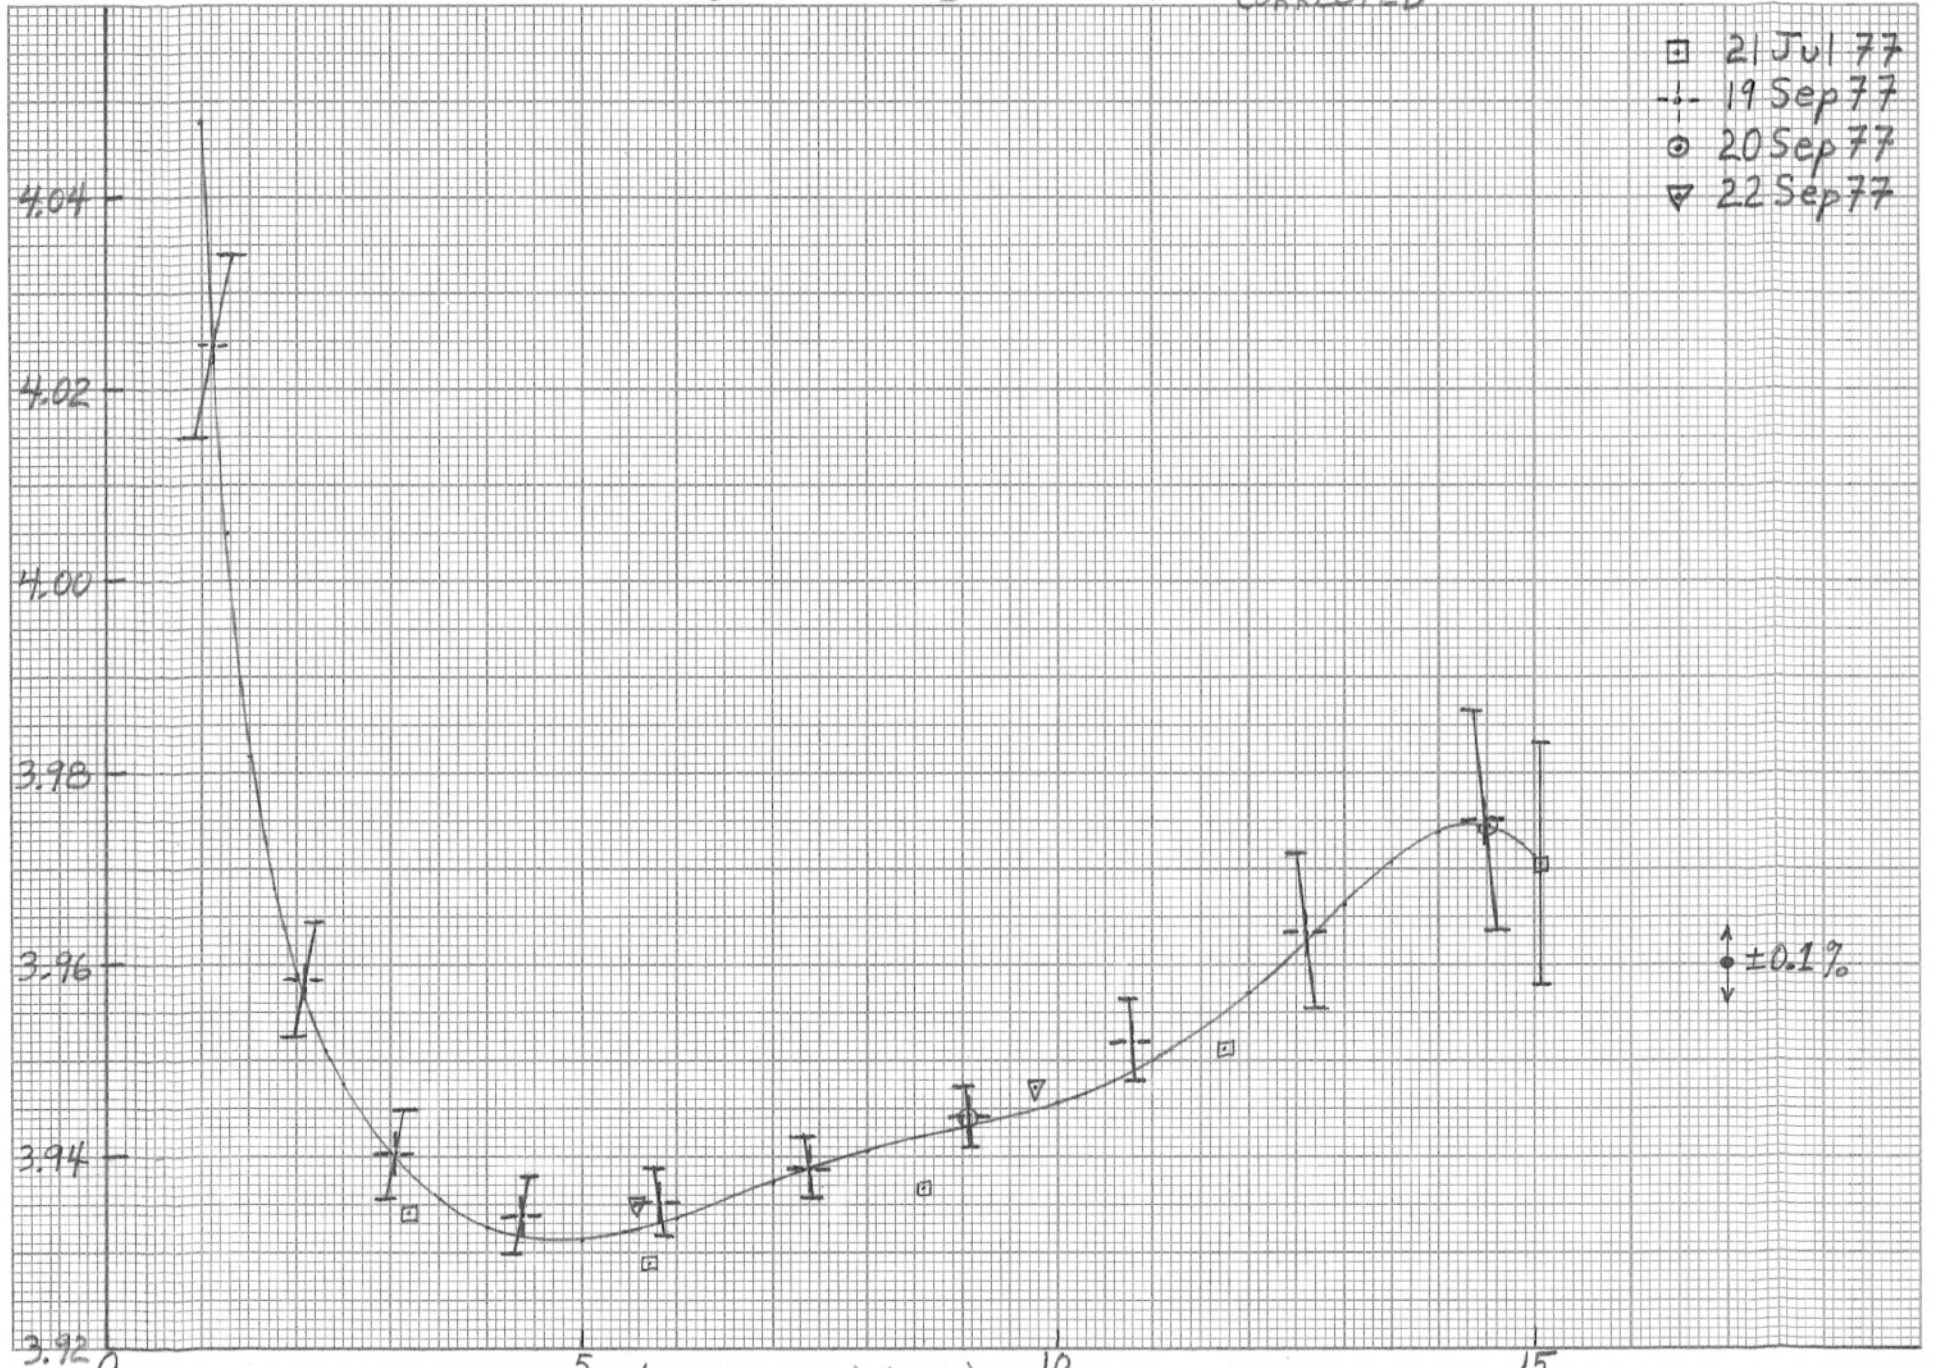


Figure 6.

(MR1-30.) (mV)

20 Apr 78

A1D6 B vs MR2 CORRECTED

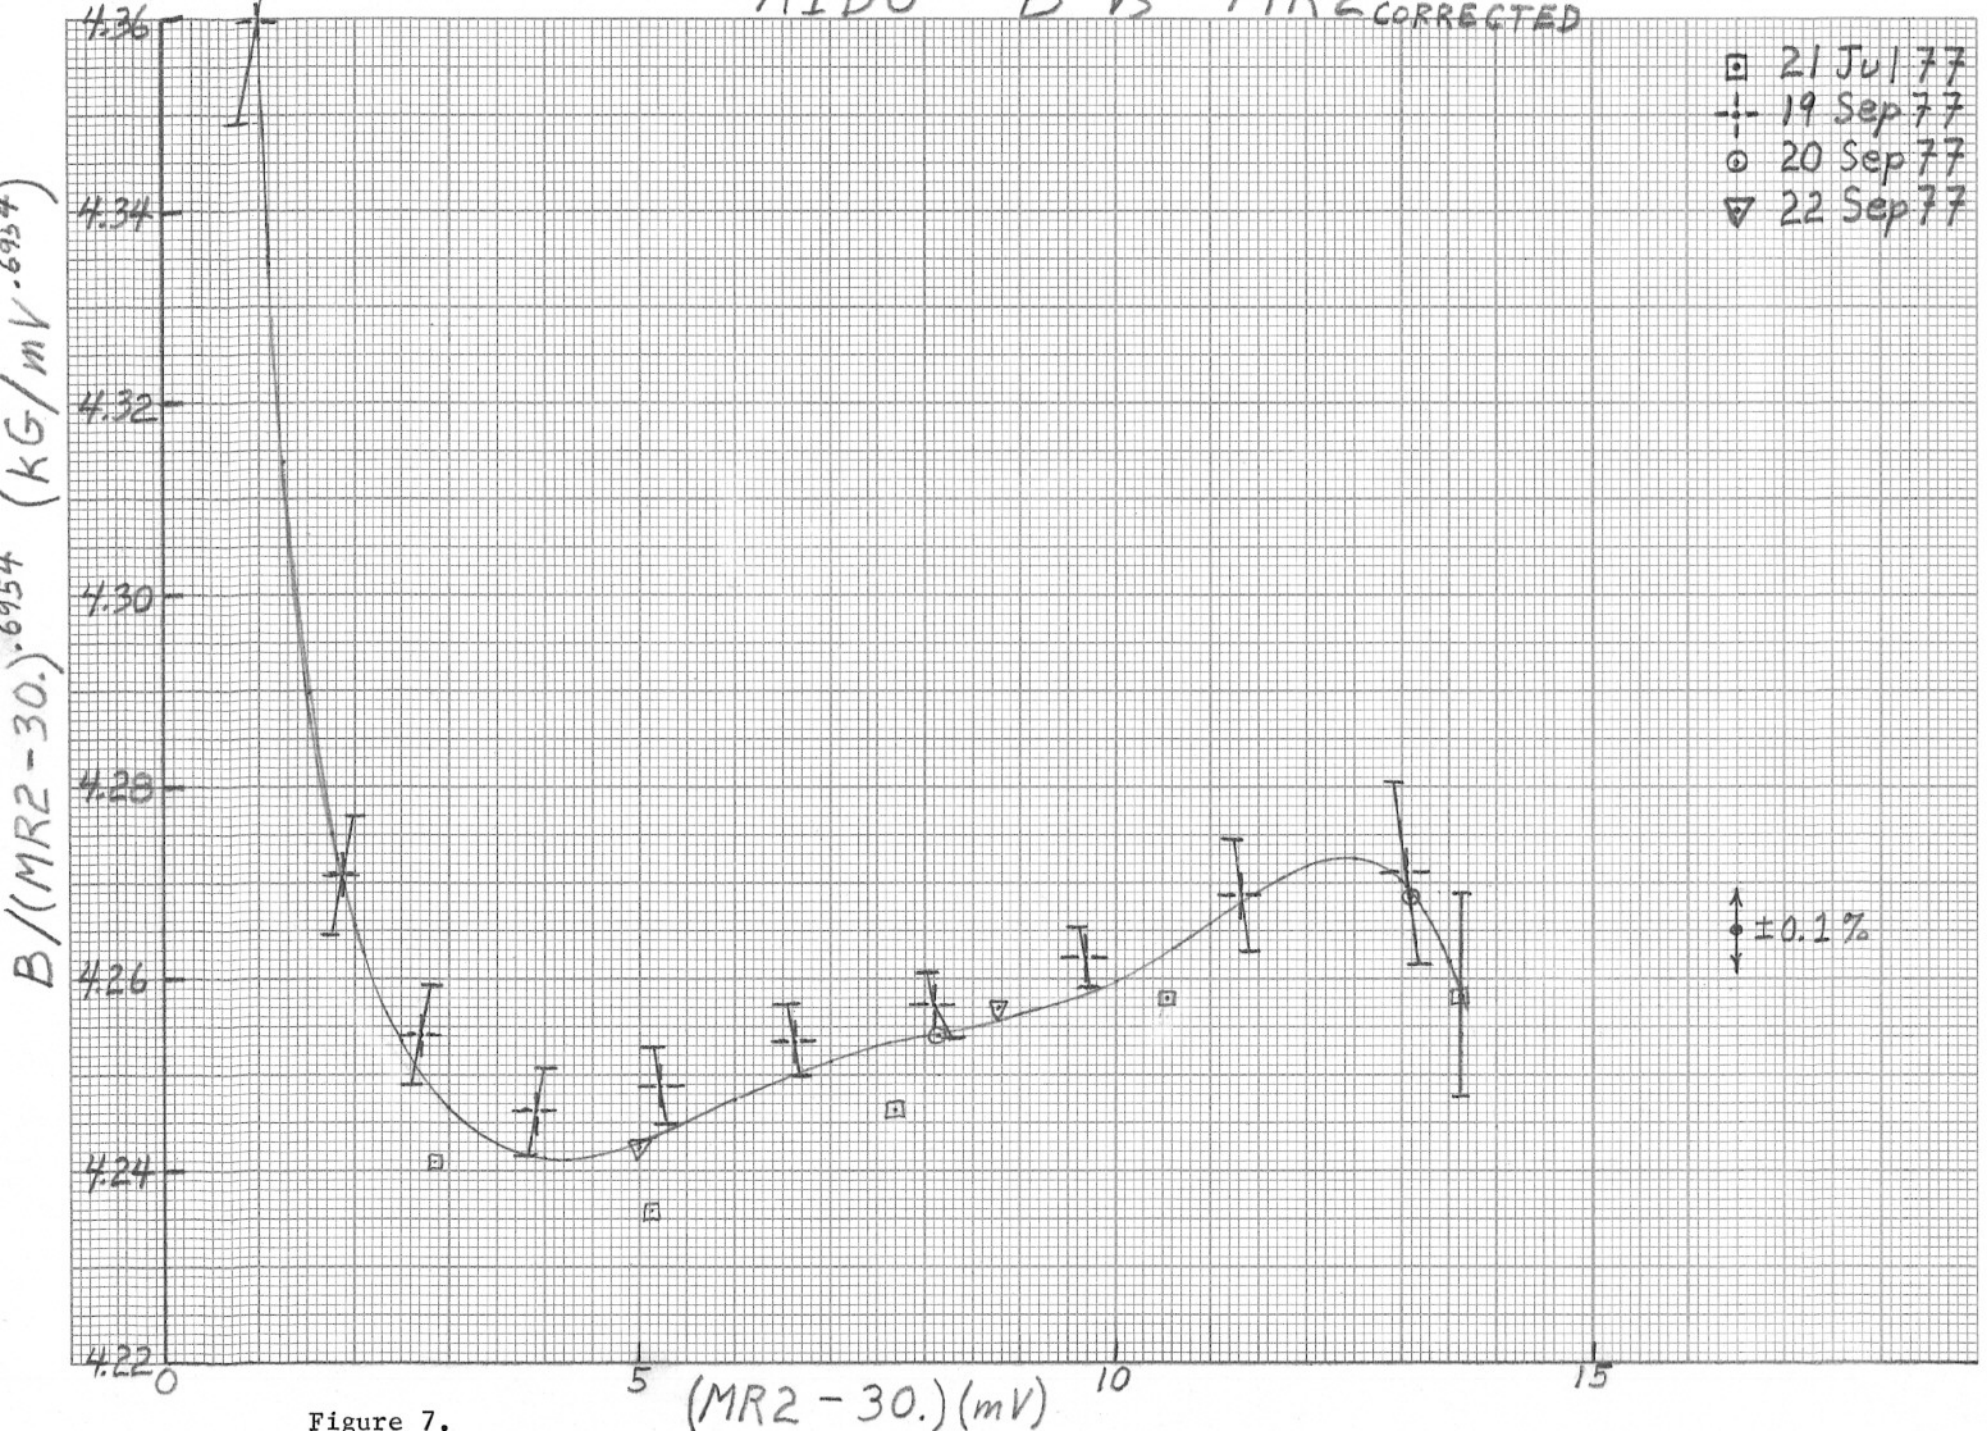


Figure 7.

20 APR 78

A1D6 B vs MR3 CORRECTED

$B / (MR3 - 30.) \cdot 6954$ (KG/mV · 6954)

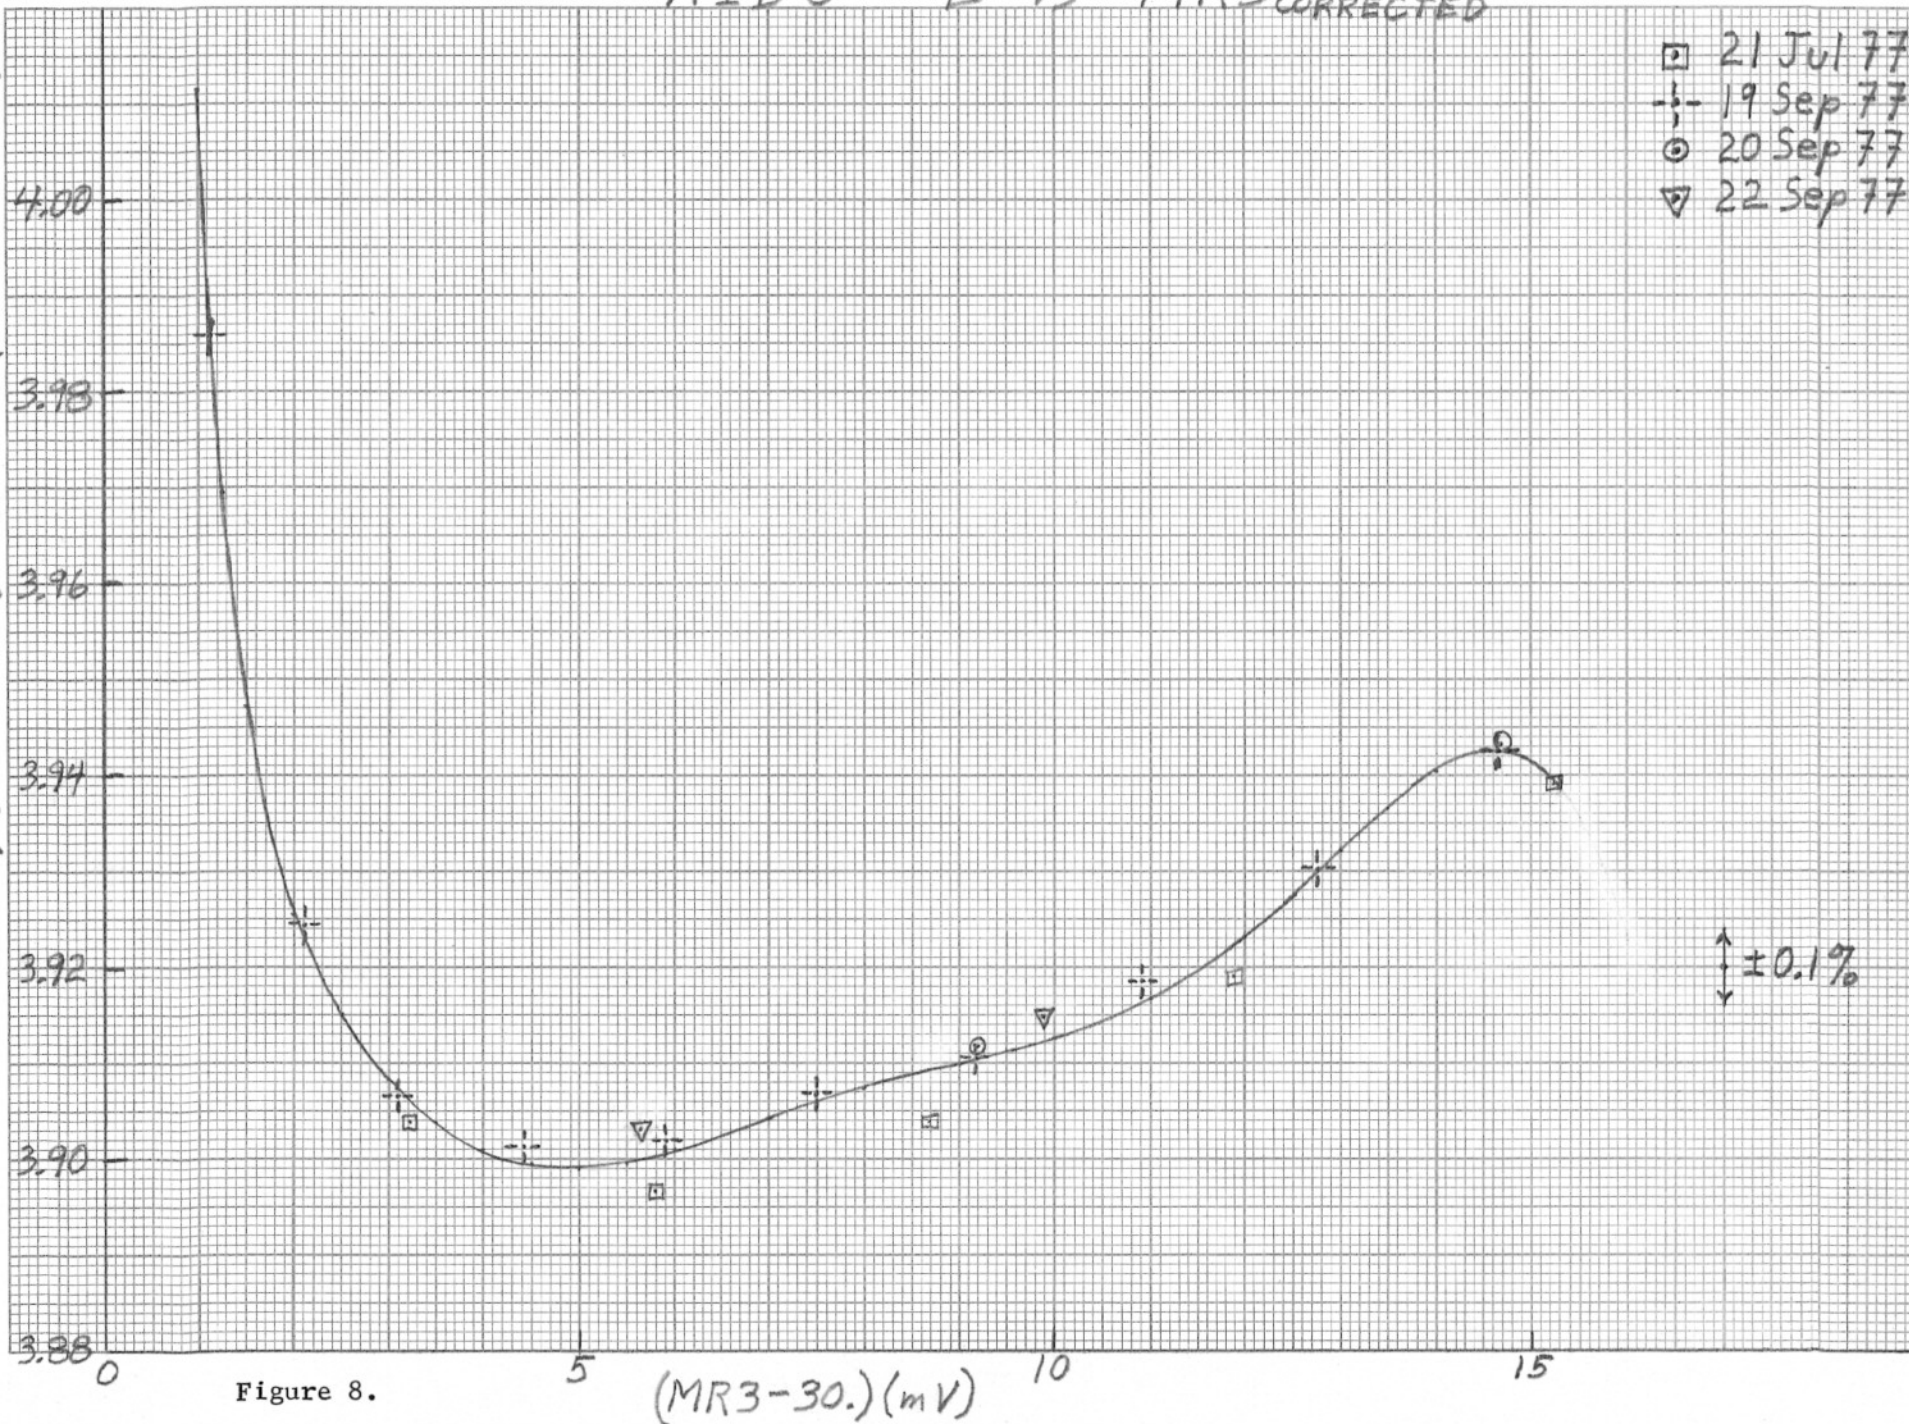


Figure 8.

Table II

A1D6

$$B = \sum_{k=0}^6 a_k (\text{MR}_{\text{corr}} - 30.)^k$$

<u>Coeff.</u>	<u>MR1</u>	<u>MR2</u>	<u>MR3</u>
a ₀	1.1771051	1.2343549	1.1687542
a ₁	3.2123958	3.5215448	3.1749166
a ₂	-.39471131	-.46639309	-.38265095
a ₃	.58125372E-1	.75758873E-1	.55075684E-1
a ₄	-.53332795E-2	-.77308508E-2	-.49462335E-2
a ₅	.26124214E-3	.42238829E-3	.23766812E-3
a ₆	-.51796952E-5	-.93749348E-5	-.46301468E-5

$$L_{\text{eff}} = \sum_{k=0}^5 c_k B^k$$

c ₀	90.31457
c ₁	-.52849413E-2
c ₂	.13692339E-2
c ₃	-.11733735E-3
c ₄	.38463944E-5
c ₅	-.39420306E-7

Effective Magnetic Lengths

(From Danby & Jackson Measurements)

$L_{eff} \equiv \int B dl / B$ (inches)

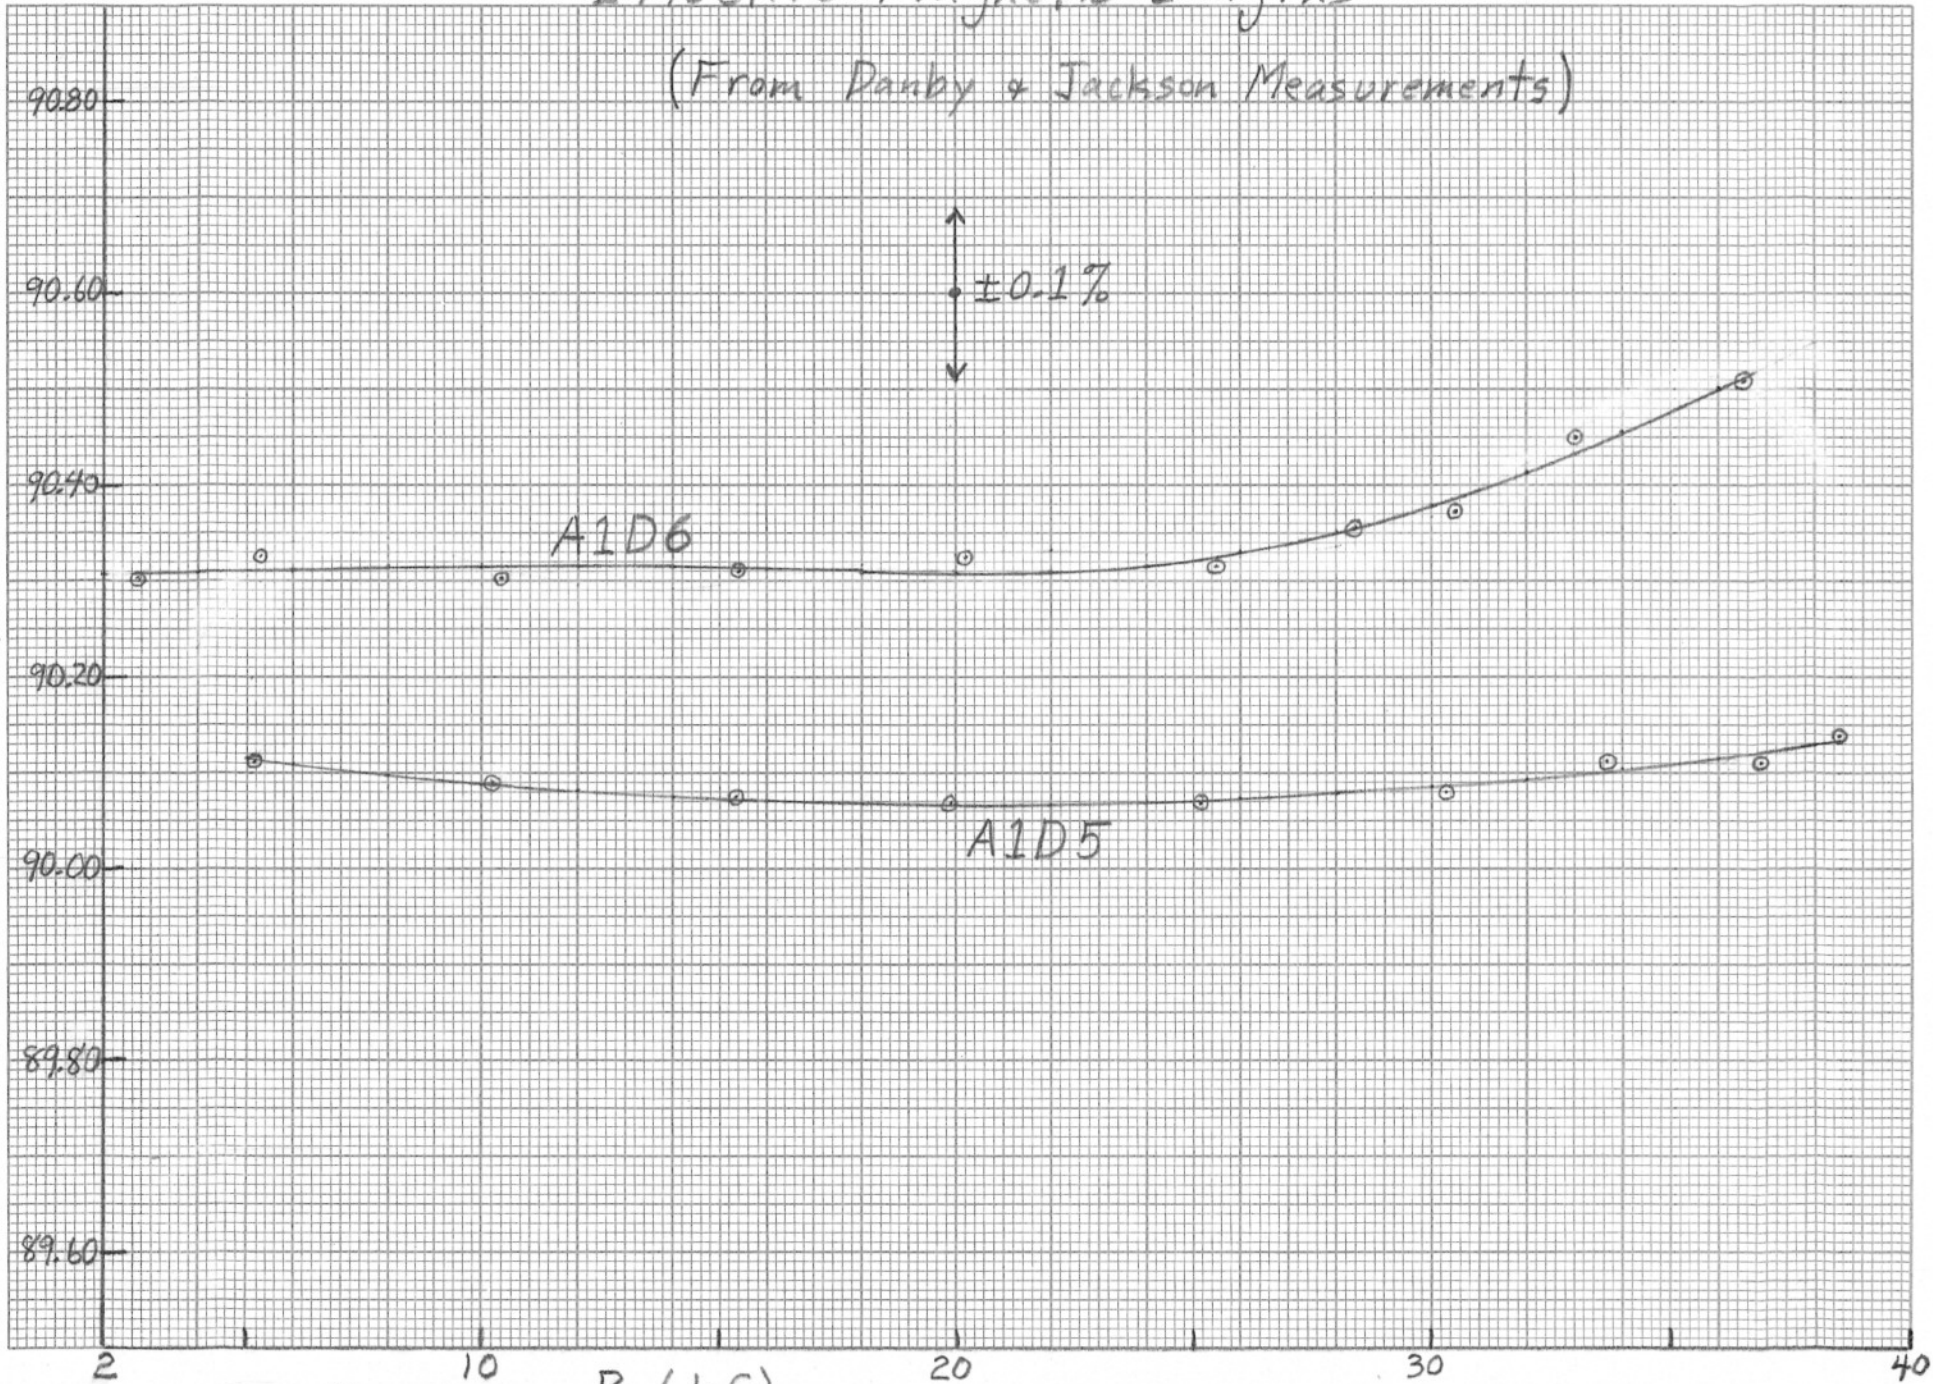


Figure 9.

B (kG)