



BNL-99267-2013-TECH

C-A/AP/115;BNL-99267-2013-IR

Booster Fault Study No. 17: Proton Beam on the D6 Septum Magnet

K. A. Brown

October 2003

Collider Accelerator Department
Brookhaven National Laboratory

U.S. Department of Energy

USDOE Office of Science (SC)

Notice: This technical note has been authored by employees of Brookhaven Science Associates, LLC under Contract No.DE-AC02-98CH10886 with the U.S. Department of Energy. The publisher by accepting the technical note for publication acknowledges that the United States Government retains a non-exclusive, paid-up, irrevocable, world-wide license to publish or reproduce the published form of this technical note, or allow others to do so, for United States Government purposes.

DISCLAIMER

This report was prepared as an account of work sponsored by an agency of the United States Government. Neither the United States Government nor any agency thereof, nor any of their employees, nor any of their contractors, subcontractors, or their employees, makes any warranty, express or implied, or assumes any legal liability or responsibility for the accuracy, completeness, or any third party's use or the results of such use of any information, apparatus, product, or process disclosed, or represents that its use would not infringe privately owned rights. Reference herein to any specific commercial product, process, or service by trade name, trademark, manufacturer, or otherwise, does not necessarily constitute or imply its endorsement, recommendation, or favoring by the United States Government or any agency thereof or its contractors or subcontractors. The views and opinions of authors expressed herein do not necessarily state or reflect those of the United States Government or any agency thereof.

C-A/AP/#115
October 2003

Booster Fault Study No. 17:
Proton Beam on the D6 Septum Magnet

K.A. Brown, C.J. Gardner
Brookhaven National Laboratory



Collider-Accelerator Department
Brookhaven National Laboratory
Upton, NY 11973

Booster Fault Study No. 17: Proton Beam on the D6 Septum Magnet

K.A. Brown and C.J. Gardner

October 8, 2003

Following is a report on the Booster fault study carried out 30 January 2003. The original fault study plan is reproduced here followed by the actual study report.

1 Study Plan

1.1 Goal

The goal of this study is to produce a primary beam loss on the D6 septum magnet and measure the resulting prompt radiation in the Booster-NSRL penetration region. Measurements are to be made on the berm over the region and in the NSRL tunnel near the penetration headwall and at the “stub” gate. The study is to be conducted in accordance with AGS OPM 9.1.9.

1.2 Initial (non-fault) Beam Conditions

1. The study is to be conducted with deuterons from Tandem or with protons from Linac.
2. The maximum kinetic energy is 1.0 GeV per nucleon for deuterons and 2.0 GeV for protons. The repetition period is at least 4 seconds.
3. The maximum intensity is 4×10^{10} deuterons or 4×10^{11} protons per Booster cycle.

1.3 Method

1. Establish beam on a Booster cycle with flat top at the desired energy. Record flat top energy and repetition period.
2. The Booster RF should be turned off just after beam reaches flat top energy. Then, as the field increases (slightly) at the end of the flat top, any surviving beam will be lost on the radially inward side of the vacuum chamber. The B6 dump bump should be adjusted so that this beam is lost on the B6 dump.
3. Establish desired intensity with no loss during flat top. Record beam current transformer trace and ring loss monitor output throughout the Booster cycle.
4. Using the flat trim windings on the C7, D1, D4, D7 and E1 dipoles, make a local distortion (bump) of the equilibrium orbit at the D6 septum magnet during the flat top portion of the magnetic cycle.
5. Adjust the amplitude of the bump so that all beam is lost on the D6 septum. A radial shift to the outside may be required.
6. Record beam current transformer trace and ring loss monitor output for the loss condition. Record output from Booster chipmunks NM134 and NM133. Record Radius and Bump parameters.
7. Measure radiation levels on the Booster berm and in the NSRL tunnel under the loss condition.

1.4 Survey Locations

Figure 1 is a schematic of the Booster-NSRL penetration region. **Figure 2** shows the actual plan view of the region. A cross-section of the berm in the area of thin soil cover is shown in **Figure 3**. The nominal cross-section of the Booster tunnel and berm is shown in **Figure 4**. Referring to these figures, the survey locations are:

1. On Booster berm directly over the D6 septum magnet. The vent shown in Figures 1 and 2 can be used as a reference point to locate the point on the berm over the D6 septum magnet. The distance between this point and the vent is some 80 feet.

2. On the berm in the area of thin soil cover indicated in Figure 1.
3. Inside the NSRL tunnel near the penetration headwall and at the stub gate indicated in Figure 1.

All surveys are to be conducted with the HP1010 meter unless otherwise noted.

1.5 Radiation Estimates

To obtain an estimate of the radiation levels we assume a point loss directly under the areas of interest and apply the formula

$$H = \frac{1}{r^2}(1.6 \times 10^{-6})Le^{-d/117} \quad (1)$$

given by Tesch [1]. Here H is the dose rate (mrem/hour) on the berm directly above the loss point, L is the loss rate (GeV/s), d is the mass-density thickness (g/cm^2) of the berm shielding, and r is the distance (meters) from the loss point.

1.5.1 On the Berm Directly over the D6 Magnet

On the berm directly over the D6 septum magnet, the depth of the soil cover is at least 427 cm (14 feet) and the distance from the magnet is $r = 5.49$ m (18 feet). Taking the density of the soil to be $1.8 \text{ g}/\text{cm}^3$, we have $d = 427 \times 1.8 = 769 \text{ g}/\text{cm}^2$. For a point loss of 10^{11} protons per second at 2 GeV kinetic energy, the dose rate on the berm would then be 15 mrem/hour. For a point loss of 10^{10} deuterons per second at 1 GeV kinetic energy per nucleon, the dose rate would be 1.5 mrem/hour.

1.5.2 On the Berm in the Area of Thin Soil Cover

Even though the loss we are considering occurs on the D6 magnet, let us assume that the loss occurs directly under the area of thin soil cover. Here the depth of the soil may be as little as 366 cm (12 feet) and the distance from the loss point may be as little as $r = 5.18$ m (17 feet). Taking the density of the soil to be $1.8 \text{ g}/\text{cm}^3$, we have $d = 366 \times 1.8 = 659 \text{ g}/\text{cm}^2$. For a point loss of 10^{11} protons per second at 2 GeV kinetic energy, the dose rate on the berm would then be 43 mr/hour. For a point loss of 10^{10}

deuterons per second at 1 GeV kinetic energy per nucleon, the dose rate would be 4.3 mr/hour. These are upper limits on the expected dose rates in the area of thin soil cover. (During the Summer of 2003 the berm in the Booster-NSRL penetration region was rebuilt and stabilized with a retaining wall. The soil cover is now at least 14 feet in this region.)

1.5.3 At the Penetration Headwall

Here, in a fault study [2] carried out on 9 December 2000, a dose rate of 7.5 mrem per hour was measured by Chipmunk NM066 which was positioned at the headwall close to the present position of Chipmunk NM134. The beam loss in this case was 1.1×10^{12} protons per second on the D6 dump at a kinetic energy of 1.74 GeV. (The D6 dump has since been removed and replaced with the D6 septum magnet.) Based on this measurement, the expected dose rate at the headwall for a loss on the D6 septum magnet of 10^{11} protons per second at 2 GeV kinetic energy would be 0.78 mrem per hour. For a loss on the septum magnet of 10^{10} deuterons per second at 1 GeV kinetic energy per nucleon, the dose rate would be a factor of ten smaller.

1.5.4 At the Stub Gate

Here the dose rate for a loss on the D6 magnet of 10^{10} deuterons per second at 1 GeV kinetic energy per nucleon has been estimated by Adam Rusek to be 0.009 mrem per hour.

2 Actual Study

2.1 Conditions

Protons from the polarized proton source (and Linac) were injected into Booster and accelerated to a kinetic energy of 1.5 GeV. Although the study plan called for a magnetic cycle with a flat top, it was more convenient to use the standard polarized proton magnetic cycle.

The magnetic cycle repetition period was $324/60 = 5.4$ seconds.

Under fault conditions all beam loss occurred approximately 108 ms from BT0 (Booster T zero) where the field was 5115 Gauss. This gives a rigidity of 7.092 Tm (assuming radius of curvature $\rho = 13.8656$ meters in the

Booster dipoles) and a kinetic energy of 1.4 GeV. The loss was 2.4×10^{11} protons per Booster cycle. With a repetition period of 5.4 seconds, this gives a loss rate of 4.4×10^{10} protons per second.

2.2 Loss Setup

The currents in the flat trim windings on dipoles C7, D1, D4, D7 and E1 were programmed to produce a local loss on the D6 septum magnet. This is shown in **Figure 5**. Here the three oscilloscope traces are the normalized beam current, the Booster main magnet current, and the current in the flat trim winding on dipole D1. The D1 trim winding current increases from 0 to +500 A in 10 ms starting 100 ms from BT0. It then decreases back to 0 in the next 10 ms. The currents in the C7, D4, D7, and E1 trim windings had the same time dependence, but with maximum amplitudes -120 , $+300$, $+500$, and $+120$ A respectively. All of the beam is lost as the currents increase to their maximum amplitudes. The time of the loss is approximately 108 ms from BT0.

2.3 Loss Measurements

Beam loss was measured with the circulating beam current transformer and with the RLM (Ring Loss Monitor) system. The loss rate determined from the beam current transformer was 4.4×10^{10} protons per second as discussed above. At a kinetic energy of 1.4 GeV, this gives an energy loss of 6.2×10^{10} GeV per second.

The RLM readings under the fault condition are listed in **Table 1**. Here the window of observation was from 100 to 120 ms from BT0 which brackets the time when beam is lost. The readings show that most of the loss occurs between the D3 and E3 straight sections with the maximum loss centered on the D6 septum magnet and the D7 dipole.

Table 1: Booster RLM Readings under Fault Condition

RLM	Counts	RLM	Counts
D1	37	F1	193
D2	74	F2	185
D3	112	F3	162
D4	2289	F4	332
D5	2196	F5	75
D6	4014	F6	1738
D7	4094	F7	1801
D8	2855	F8	192
E1	2251	A1	94
E2	2170	A2	162
E3	424	A3	23
E4	18	A4	80
E5	203	C5	121
E6	734	C6	188
E7	496	C7	215
E8	241	C8	98

2.4 Radiation Measurements

Radiation measurements were made with the HP1010 meter and the E600 “rem ball”. The levels were also monitored by Chipmunks NM133 and NM134. The positions of the chipmunks are shown in **Figure 1**. NM134 is mounted on the stub tunnel headwall near the beampipe. NM133 is mounted on the wall near the stub tunnel gate.

2.4.1 On the Berm over the D6 Septum Magnet

Here the HP1010 meter and E600 rem ball were placed on the ground and gave readings that are summarized in **Table 2**. The measured dose rate due to the fault is 0.112 mrem per hour. For a point loss of 10^{11} protons per second at 2 GeV kinetic energy, the predicted dose rate is 15 mrem/hour. The predicted dose rate for a point loss of 4.4×10^{10} protons per second at 1.4 GeV kinetic energy is then $1.4 \times 4.4 \times 15/20 = 4.6$ mrem per hour. This is 41 times higher than the observed dose rate.

Table 2: Radiation Levels on the Berm over the D6 Septum Magnet

<u>Condition</u>	<u>Meter</u>	<u>Dose Rate</u> (mrem/h)
Fault	HP1010	< 0.05
	E600	0.183
Beam Off	HP1010	< 0.05
	E600	0.071

2.4.2 In the Stub Tunnel and at the Stub Gate

Here the E600 rem ball was placed on the floor in the stub tunnel downstream of the headwall and upstream of the concrete blocks shown in Figure 1. The HP1010 meter was held by a technician standing at the stub gate. The readings from both devices are summarized in **Table 3**.

Table 3: Radiation Levels in the Stub Tunnel and at the Stub Gate

<u>Condition</u>	<u>Location</u>	<u>Meter</u>	<u>Dose Rate</u> (mrem/h)
Fault	Tunnel	E600	0.425
	Gate	HP1010	0.05
Beam Off	Tunnel	E600	0.062
	Gate	HP1010	0.05

Here we see that the dose rate in the stub tunnel due to the fault is 0.363 mrem per hour. At the gate the HP1010 meter registered no discernable difference between the beam off and fault conditions.

As discussed in Section 1.5.3, the expected dose rate at the headwall for a loss on the D6 septum magnet of 10^{11} protons per second at 2 GeV kinetic energy is 0.78 mrem per hour. The expected dose rate for a loss of 4.4×10^{10} protons per second at 1.4 GeV kinetic energy is then 0.24 mrem per hour. This is in good agreement with the observed rate of 0.363 mrem per hour.

2.4.3 Chipmunks

Chipmunk NM134 (mounted on the headwall near the beampipe) registered a dose rate of 0.35 mrem per hour due to the fault. This is in good agreement with the E600 rem ball measurements in Table 3.

Chipmunk NM133 (mounted on the wall near the gate) registered a dose rate of 0.15 mrem per hour due to the fault.

References

- [1] K. Tesch, Health Physics, Vol. 44, No. 1, pp. 79–82, January, 1983.
- [2] C. J. Gardner, “Booster Fault Study for the BAF Penetration Site”, AGS Studies Report 375, January 13, 2000.

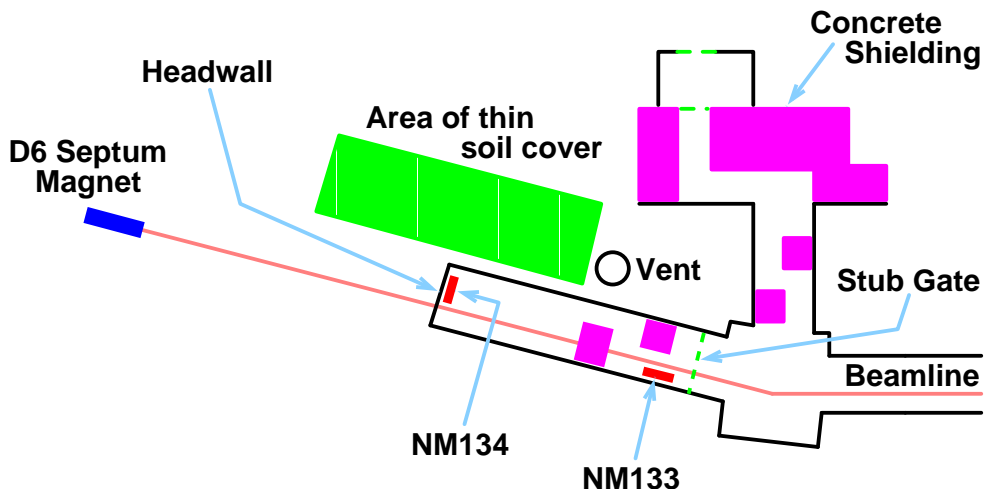


Figure 1: Schematic of the Booster-NSRL penetration region. The stub tunnel is the area between the headwall and the stub gate. Radiation measurements are to be taken on top of the berm directly over the D6 septum magnet and on the side of the berm in the area of thin soil cover. Measurements also are to be taken in the tunnel near the headwall and at the stub gate.

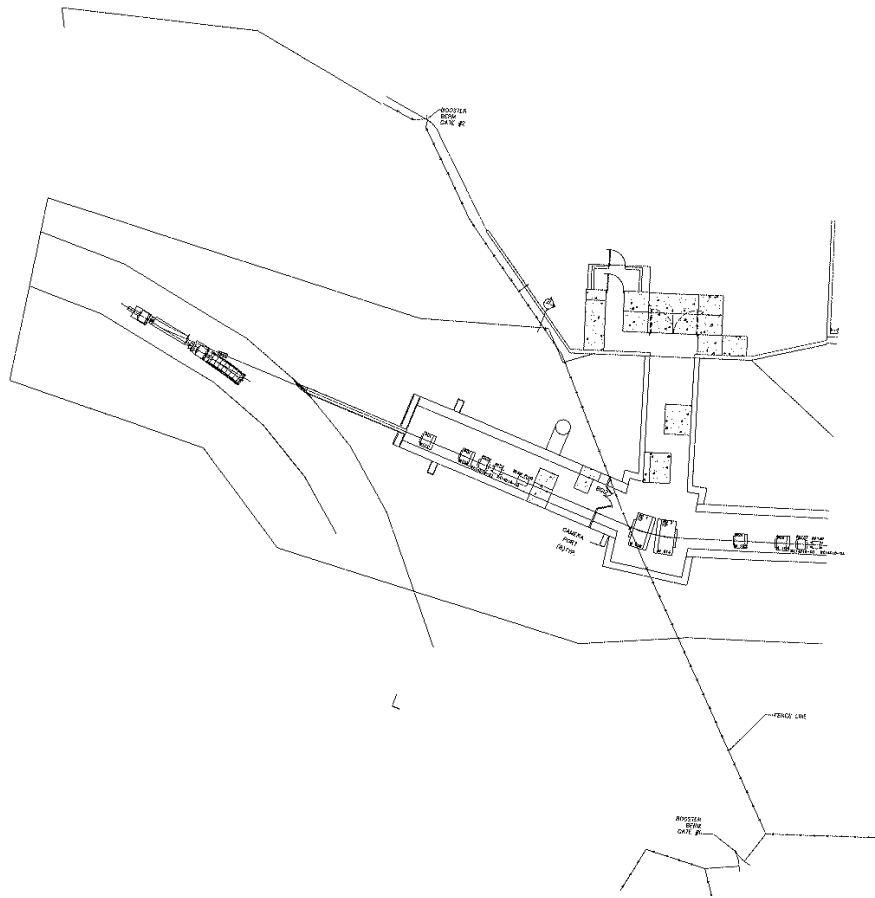


Figure 2: Plan view of Booster-NSRL penetration region. This is from drawing number 82000002.

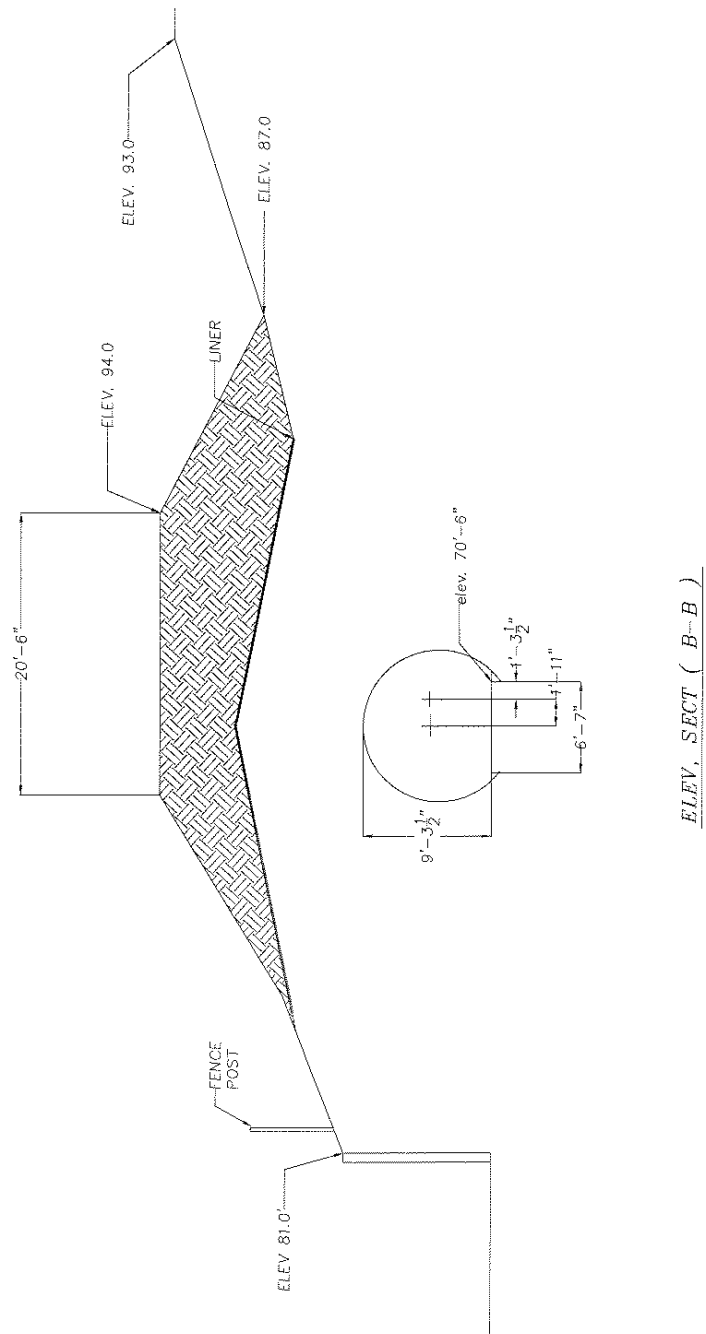


Figure 3: Cross-section of berm in the area of thin soil cover. This is cross-section B from drawing number 82000002.

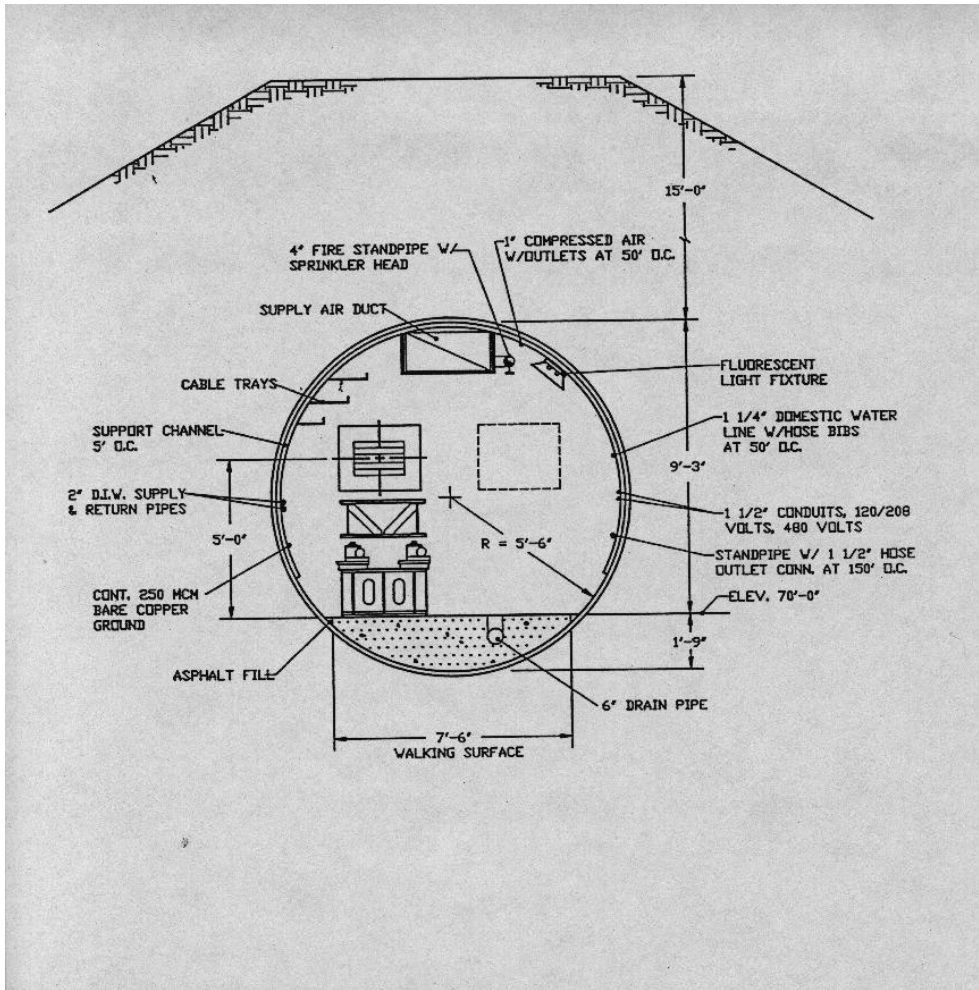


Figure 4: Nominal cross-section of Booster tunnel and berm. This is from the Ags Booster Final Safety Analysis Report, February 27, 1991. Note that the elevation of the tunnel floor is 70 feet. The center of the beam pipe is 5 feet above the floor and the top of the tunnel is 9 feet 3 inches above the floor. The nominal depth of soil over the tunnel is 15 feet.

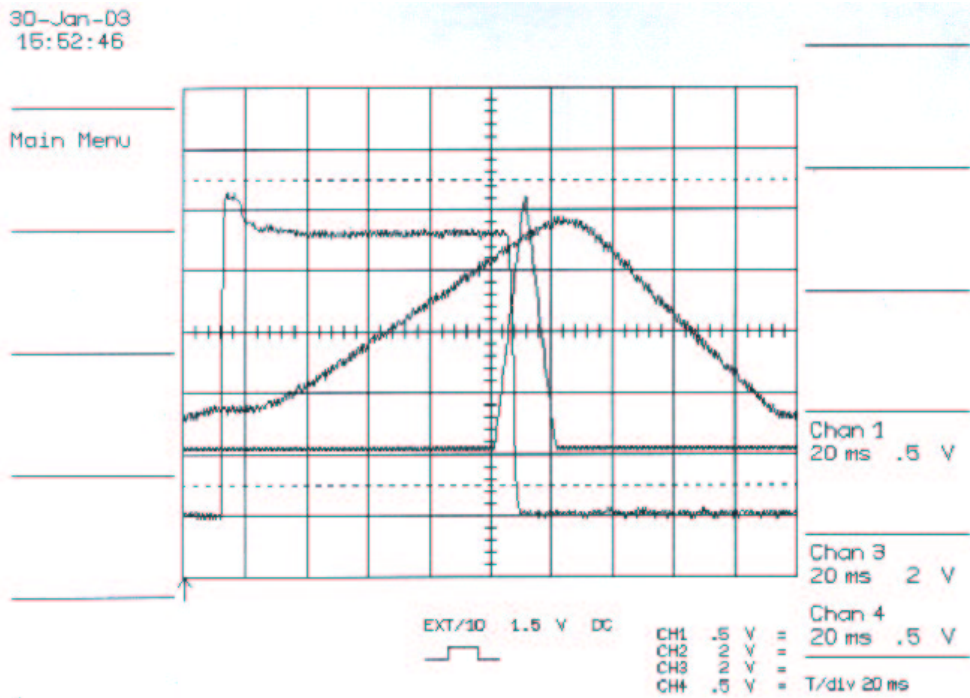


Figure 5: Fault study loss setup. Here the three oscilloscope traces are the normalized beam current, the Booster main magnet current, and the current in the flat trim winding on dipole D1. The trim winding current increases from 0 to 500 A in 10 ms starting 100 ms from BT0. It then decreases back to 0 in the next 10 ms. All of the beam is lost as the current increases to 500 A. The loss time is approximately 108 ms from BT0.