

BNL-101452-2014-TECH RHIC/RF- 33;BNL-101452-2013-IR

## Analysis of beampipe transitions for the RHIC RF cavities

#### S. Kwiatkowski

June 1996

Collider Accelerator Department

Brookhaven National Laboratory

## **U.S. Department of Energy**

USDOE Office of Science (SC)

Notice: This technical note has been authored by employees of Brookhaven Science Associates, LLC under Contract No.DE-AC02-76CH00016 with the U.S. Department of Energy. The publisher by accepting the technical note for publication acknowledges that the United States Government retains a non-exclusive, paid-up, irrevocable, world-wide license to publish or reproduce the published form of this technical note, or allow others to do so, for United States Government purposes.

#### **DISCLAIMER**

This report was prepared as an account of work sponsored by an agency of the United States Government. Neither the United States Government nor any agency thereof, nor any of their employees, nor any of their contractors, subcontractors, or their employees, makes any warranty, express or implied, or assumes any legal liability or responsibility for the accuracy, completeness, or any third party's use or the results of such use of any information, apparatus, product, or process disclosed, or represents that its use would not infringe privately owned rights. Reference herein to any specific commercial product, process, or service by trade name, trademark, manufacturer, or otherwise, does not necessarily constitute or imply its endorsement, recommendation, or favoring by the United States Government or any agency thereof or its contractors or subcontractors. The views and opinions of authors expressed herein do not necessarily state or reflect those of the United States Government or any agency thereof.

# RHIC Project BROOKHAVEN NATIONAL LABORATORY

RHIC/RF Technical Note No. 33

# ANALYSIS OF BEAMPIPE TRANSITIONS FOR THE RHIC rf CAVITIES

S. Kwaitkowski, C. Quiery, J. Rose

## Analysis of Beampipe Transitions for the RHIC rf Cavities S. Kwiatkowski, C. Quiery, J. Rose

#### Introduction

BNL RHIC facility has two 3.8km long synchrotrons able to accept protons or heavy ions beam from AGS, accelerate them to final energy (250GeV/n for protons and 100GeV/n for fully stripped gold) and store for several hours. Each accelerating system consists two quarterwave cavities placed back to back and connected with use of stainless bellows. The inner diameter of the beam pipe inside the 28MHz prototype cavity changes from 6.2 cm(accelerating gap area) to 12cm (an inner diameter of the beam pipe inside the 28MHz prototype cavity). The topic of this analysis is to find out how harmful trapped modes in the inner conductor volume could be for the accelerating beam.

### 1. Accelerating Cavity Longitudinal modes.

Since the cutoff frequency of the cylindrical waveguide with the radius 6.2cm for  $TM_{01}$  mode is 1847MHz and the first possible resonance ( $E_{010}$ ) in 12 cm pipes is 950 MHZ there will be many resonances trapped inside the inner conductors of the 28MHz accelerating cavities. The cross section of the inner conductor of the prototype cavity is shown in Fig.1. The analysis is performed on the trapped volume of a cavity pair and so the results shown are per ring (two cavities per ring).

The first modes have the indexes'  $E_{010}$  to  $E_{01n}$ , since the length of the involuntary formed cavity (2.2m) is much longer than the diameter. First 10 longitudinal modes have been calculated using URMEL code and the results are given in Table 1.

MODE No.	Frequency [MHZ]	Rsh [kΩ]	Qo[]	R/Q [Ω]
1	951	560	40870	13.7
2	958	175	51470	3.4
3	966	8	50000	0.16
4	979	466	48500	9.6
5	996	47	48450	0.97
6	1018	37	48680	0.76
7	1044	537	49270	10.9
8	1074	139	49820	2.79
9	1108	1	50000	0.002
10	1144	8	50000	1.6

TABLE 1.

The impedance limit for 28MHz accelerating cavity longitudinal modes have been determined [1]. Figure 2 shows the beam pipe longitudinal modes plotted against the impedance limit curve.

#### 2. Accelerating Cavity Perpendicular modes.

The longitudinal impedance of the first twenty dipole modes has been calculated using the code URMEL. The transverse impedance was then calculated as

$$R \perp = \frac{2 * c * R \parallel}{a^2 * \omega}$$

where R | is integrated at the beampipe radius "a".

The results (for the modes with the  $R_{\perp} > 100 \text{k}\Omega/\text{m}$ ) are given in Table 2.

Mode No	Frequency [MHZ]	R <sub>⊥</sub> [MΩ/m]	Q[]
9	962	0.24	53700
10	1008	0.3	57400
13	1159	0.13	69300
15	1267	0.2	75800
16	1322	2.84	77800
17	1385	12.99	58600
18	1409	8.87	57200
19	1435	6.17	85900

Table 2

## 3) Storage Cavity interconnects

The HOM impedances of the 197.1 MHZ storage cavities has been described elsewhere in detail [2], [3]. There is however, a trapped volume in the interconnect region between either adjacent cavities or between the cavities and the 5 inch RHIC beampipe which can support HOM's. This geometry is shown in figure 3. The step is only a little over 10 mm in radius and should have little or no effect on the beam. It is therefore recommended that no taper be installed to simplify the interconnect region and eliminate unnecessary vacuum seals. If analysis or beam measurements show that this step is harmful to the beam a liner can be installed at a later date.

## **Conclusion:**

There is no danger for the accelerating beam coming from the longitudinal HOM's trapped inside the inner conductor of the 28MHz cavity, however the transverse impedances are very strong and may lead to transverse instabilities, either bunch to bunch or head/tail. Since the cost of the "liner" (device which will keep the diameter of the beam pipe inside the 28 MHZ constant and equal 12.4 cm) is only 1% of the cost of the accelerating cavity it is recommended to apply it.

#### **References:**

- [1] "Coupled Bunch Instabilities and Implications for RHIC rf Cavity Impedances" J. Rose, RHIC/rf-27
- [2] Ibidem
- [3] "A New Type of Broadband Higher Order Mode Coupler Using Parallel Ridged Waveguide In Comparison with a Coaxial Filter Version" F. Caspers, G. Dome, H. R. Kinderman IEEE PAC, 1987

## Analysis of Beampipe Transitions for the RHIC rf Cavities S. Kwiatkowski, C. Quiery, J. Rose

#### Introduction

BNL RHIC facility has two 3.8km long synchrotrons able to accept protons or heavy ions beam from AGS, accelerate them to final energy (250GeV/n for protons and 100GeV/n for fully stripped gold) and store for several hours. Each accelerating system consists two quarterwave cavities placed back to back and connected with use of stainless bellows. The inner diameter of the beam pipe inside the 28MHz prototype cavity changes from 6.2 cm(accelerating gap area) to 12cm (an inner diameter of the beam pipe inside the 28MHz prototype cavity). The topic of this analysis is to find out how harmful trapped modes in the inner conductor volume could be for the accelerating beam.

## 1. Accelerating Cavity Longitudinal modes.

Since the cutoff frequency of the cylindrical waveguide with the radius  $6.2 \, \mathrm{cm}$  for  $TM_{01}$  mode is 1847MHz and the first possible resonance ( $E_{010}$ ) in 12 cm pipes is 950 MHZ there will be many resonances trapped inside the inner conductors of the 28MHz accelerating cavities. The cross section of the inner conductor of the prototype cavity is shown in Fig.1. The analysis is performed on the trapped volume of a cavity pair and so the results shown are per ring (two cavities per ring).

The first modes have the indexes'  $E_{010}$  to  $E_{01n}$ , since the length of the involuntary formed cavity (2.2m) is much longer than the diameter. First 10 longitudinal modes have been calculated using URMEL code and the results are given in Table 1.

MODE No.	Frequency [MHZ]	Rsh [kΩ]	Qo [ ]	R/Q [Ω]
1	951	560	40870	13.7
2	958	175	51470	3.4
3	966	8	50000	0.16
4	979	466	48500	9.6
5	996	47	48450	0.97
6	1018	37	48680	0.76
7	1044	537	49270	10.9
8	1074	139	49820	2.79
9	1108	1	50000	0.002
10	1144	8	50000	1.6

TABLE 1.

The impedance limit for 28MHz accelerating cavity longitudinal modes have been determined [1]. Figure 2 shows the beam pipe longitudinal modes plotted against the impedance limit curve.

## 2. Accelerating Cavity Perpendicular modes.

The longitudinal impedance of the first twenty dipole modes has been calculated using the code URMEL. The transverse impedance was then calculated as

$$R\perp = \frac{2*c*R\parallel}{a^2*\omega}$$

where R | is integrated at the beampipe radius "a".

The results (for the modes with the  $R_{\perp} > 100 \text{k}\Omega/\text{m}$ ) are given in Table 2.

Mode No	Frequency [MHZ]	R <sub>⊥</sub> [MΩ/m]	Q[]
9	962	0.24	53700
10	1008	0.3	57400
13	1159	0.13	69300
15	1267	0.2	75800
16	1322	2.84	77800
17	1385	12.99	58600
18	1409	8.87	57200
19	1435	6.17	85900

Table 2

## 3) Storage Cavity interconnects

The HOM impedances of the 197.1 MHZ storage cavities has been described elsewhere in detail [2], [3]. There is however, a trapped volume in the interconnect region between either adjacent cavities or between the cavities and the 5 inch RHIC beampipe which can support HOM's. This geometry is shown in figure 3. The step is only a little over 10 mm in radius and should have little or no effect on the beam. It is therefore recommended that no taper be installed to simplify the interconnect region and eliminate unnecessary vacuum seals. If analysis or beam measurements show that this step is harmful to the beam a liner can be installed at a later date.

#### **Conclusion:**

There is no danger for the accelerating beam coming from the longitudinal HOM's trapped inside the inner conductor of the 28MHz cavity, however the transverse impedances are very strong and may lead to transverse instabilities, either bunch to bunch or head/tail. Since the cost of the "liner" (device which will keep the diameter of the beam pipe inside the 28 MHZ constant and equal 12.4 cm) is only 1% of the cost of the accelerating cavity it is recommended to apply it.

#### References:

- [1] "Coupled Bunch Instabilities and Implications for RHIC rf Cavity Impedances" J. Rose, RHIC/rf-27
- [2] Ibidem
- [3] "A New Type of Broadband Higher Order Mode Coupler Using Parallel Ridged Waveguide In Comparison with a Coaxial Filter Version" F. Caspers, G. Dome, H. R. Kinderman IEEE PAC, 1987

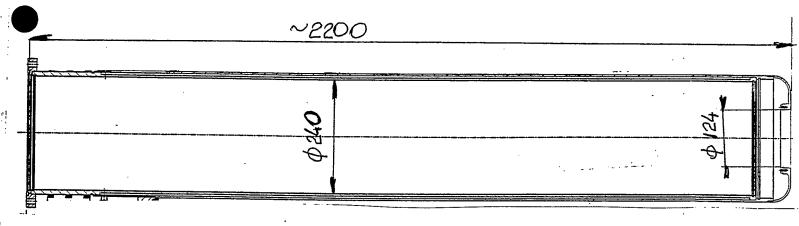


Fig. 1

Short the file of the contract

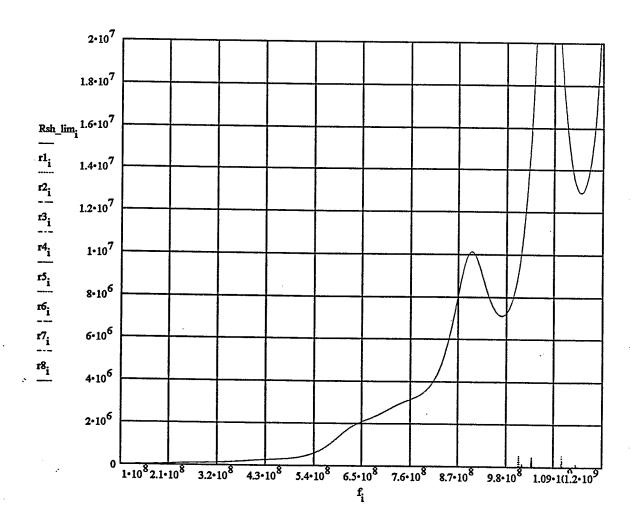


Fig. 2.

